


End Product Testing Algorithm USP <797>

Do I Perform a Sterility Test?

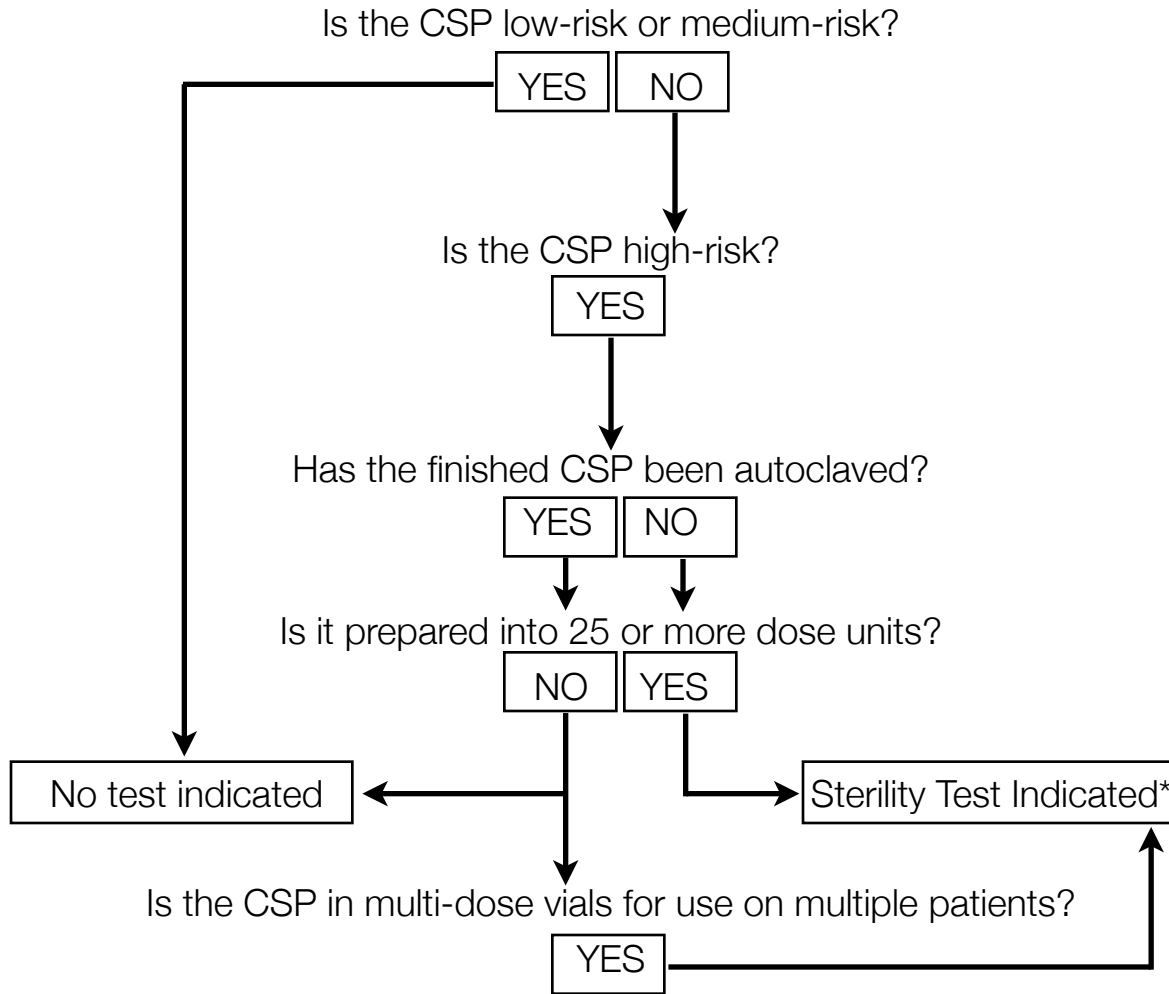

Do I Perform an Endotoxin Test?

Follow the same algorithm unless the CSP is intended for topical ophthalmic or inhalation use.

* This algorithm only applies to CSPs (once completed) that have not been exposed to temperatures of :
2-8 °C for 12 hours or longer
> 8 °C for 6 hours or longer.

If exposed to these conditions, a sterility test must be conducted.