



US012035930B2

(12) **United States Patent**
Nicholson et al.

(10) **Patent No.:** **US 12,035,930 B2**
(45) **Date of Patent:** ***Jul. 16, 2024**

(54) **REENTRY CATHETER FOR CROSSING A VASCULAR OCCLUSION**

(71) Applicant: **Traverse Vascular, Inc.**, Solana Beach, CA (US)

(72) Inventors: **Bill Nicholson**, York, PA (US); **Brad Klos**, Solana Beach, CA (US); **Steve Howard**, La Jolla, CA (US); **David Matsuura**, Solana Beach, CA (US)

(73) Assignee: **Traverse Vascular, Inc.**, Solana Beach, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 288 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **17/452,118**

(22) Filed: **Oct. 25, 2021**

(65) **Prior Publication Data**

US 2022/0110645 A1 Apr. 14, 2022

Related U.S. Application Data

(63) Continuation of application No. 16/838,863, filed on Apr. 2, 2020, now Pat. No. 11,154,312.

(Continued)

(51) **Int. Cl.**

A61B 17/22 (2006.01)

A61F 2/82 (2013.01)

(Continued)

(52) **U.S. Cl.**

CPC **A61B 17/22** (2013.01); **A61F 2/82** (2013.01); **A61F 2/958** (2013.01);

(Continued)

(58) **Field of Classification Search**

CPC A61B 17/22; A61B 2017/22002; A61B 2017/22038; A61B 2017/22071;

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,065,018 A 6/1913 Barber
1,383,683 A 7/1921 William

(Continued)

FOREIGN PATENT DOCUMENTS

CN 107260252 A 10/2017
DE 19634866 3/1998

(Continued)

OTHER PUBLICATIONS

Response to Office Action filed Jul. 20, 2023, in U.S. Appl. No. 16/838,841.

(Continued)


Primary Examiner — Richard G Louis

(74) *Attorney, Agent, or Firm* — Dorsey & Whitney LLP

(57) **ABSTRACT**

A reentry catheter for crossing a vascular occlusion includes an elongate flexible tubular body, having a proximal end, a distal end and at least one lumen extending there through. A reentry zone on the tubular body includes at least two and preferably three sets of opposing pairs of axially spaced exit apertures in communication with the lumen. The apertures are rotationally offset from each other and aligned in a spiral pattern around the tubular body. Each aperture may be defined within a radiopaque reinforcing ring embedded within the tubular body. A first set of opposing pairs of reinforcing rings may be separated axially from a second set of opposing pairs of reinforcing rings and may be connected by a flexible hinge section.

13 Claims, 21 Drawing Sheets

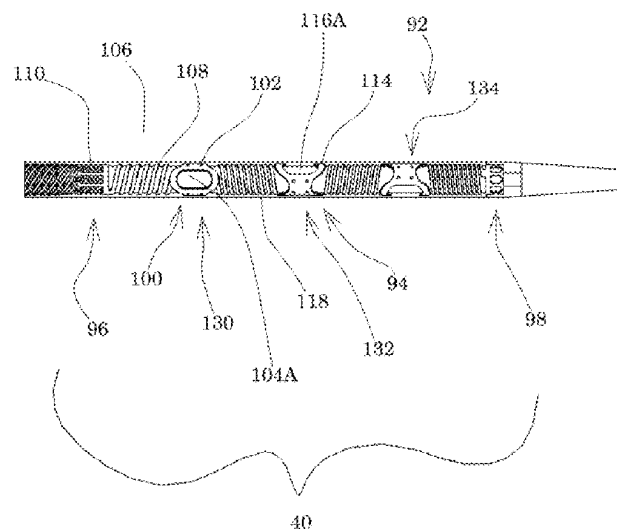

9,233,224	B1	1/2016	Pursley	
9,259,340	B2	2/2016	Heuser et al.	
9,301,774	B2	4/2016	O'day	
9,486,239	B2	11/2016	Anderson et al.	
9,867,530	B2	1/2018	Pursley	
9,872,685	B2	1/2018	Kugler et al.	
9,878,128	B2	1/2018	Kugler et al.	
10,065,018	B2	9/2018	Rocha-Singh et al.	
10,070,877	B2	9/2018	Warren	
10,117,659	B2	11/2018	Zhou et al.	
10,172,632	B2	1/2019	Morero et al.	
10,226,602	B1	3/2019	Panian	
10,226,603	B1	3/2019	Panian	
10,265,206	B2	4/2019	Heuser et al.	
10,335,174	B2	7/2019	Wilkinson	
10,456,252	B2	10/2019	Simon et al.	
10,456,557	B2	10/2019	Guala et al.	
10,603,467	B2	3/2020	Alvarez et al.	
10,610,669	B2	4/2020	Rocha-Singh et al.	
10,682,502	B2	6/2020	Panian	
10,722,252	B2	7/2020	Brenizer et al.	
10,806,474	B2	10/2020	Kugler et al.	
10,806,487	B2	10/2020	Kugler et al.	
10,857,329	B2	12/2020	Davies et al.	
10,864,041	B2	12/2020	Urbanski et al.	
10,939,928	B2	3/2021	Kugler et al.	
10,980,552	B2	4/2021	Mustapha	
11,033,286	B2	6/2021	Anderson	
11,065,002	B2	7/2021	Kugler et al.	
11,154,312	B2	10/2021	Nicholson et al.	
11,298,511	B2	4/2022	Kugler et al.	
11,369,392	B2	6/2022	Nicholson et al.	
11,602,362	B2	3/2023	Nicholson et al.	
2001/0016729	A1	8/2001	Divino et al.	
2002/0103459	A1	8/2002	Sparks et al.	
2002/0169436	A1	11/2002	Gurm et al.	
2003/0045842	A1	3/2003	Kawakita	
2004/0133158	A1	7/2004	Keith et al.	
2005/0154442	A1	7/2005	Eidenschink et al.	
2006/0276749	A1	12/2006	Selmon et al.	
2007/0010840	A1	1/2007	Rosenthal et al.	
2008/0009804	A1 *	1/2008	Rosetti	A61M 25/0029 604/173
2008/0154172	A1	6/2008	Mauch	
2009/0043372	A1	2/2009	Northrop	
2009/0112153	A1	4/2009	Gregersen	
2009/0177119	A1	7/2009	Heidner	
2009/0192435	A1	7/2009	Gregersen	
2010/0063479	A1	3/2010	Merdan	
2010/0063534	A1	3/2010	Kugler	
2010/0076404	A1	3/2010	Ring	
2010/0191279	A1	7/2010	Kassab et al.	
2010/0286718	A1	11/2010	Kassab et al.	
2011/0054448	A1	3/2011	Bourne et al.	
2011/0144677	A1	6/2011	Ward et al.	
2011/0224666	A1	9/2011	Davies et al.	
2012/0095485	A1	4/2012	Cully et al.	
2012/0179144	A1	7/2012	Carleo	
2012/0184977	A1	7/2012	Wolf	
2013/0006173	A1	1/2013	Alvarez et al.	
2013/0072957	A1	3/2013	Anderson	
2013/0085477	A1	4/2013	Deshpande	
2013/0197353	A1	8/2013	Von Oepem	
2013/0245430	A1	9/2013	Selmon	
2013/0304108	A1	11/2013	Weber et al.	
2013/0317528	A1	11/2013	Anderson et al.	
2014/0074108	A1 *	3/2014	Warren	A61M 25/104 606/108
2014/0155862	A1	6/2014	Baxter et al.	
2014/0228876	A1	8/2014	Copeta	
2014/0275983	A1	9/2014	Piccagli	
2015/0112374	A1	4/2015	Wilkinson	
2015/0174371	A1	6/2015	Schaeffer et al.	
2016/0045714	A1	2/2016	Zhou et al.	
2016/0074627	A1 *	3/2016	Cottone	A61M 25/0194 604/510
2017/0020563	A1	1/2017	Anderson et al.	
2017/0021127	A1	1/2017	Manouchehr et al.	
2017/0100141	A1	4/2017	Morera	

(56)

References Cited**U.S. PATENT DOCUMENTS**

2017/0246427	A1	8/2017	Gurley
2017/0281909	A1	10/2017	Northrop
2018/0036021	A1	2/2018	Kassab
2018/0056045	A1	3/2018	Donoghue et al.
2018/0056046	A1	3/2018	Kiersey et al.
2018/0110525	A1	4/2018	Kugler et al.
2018/0333162	A1	11/2018	Saab
2018/0369539	A1	12/2018	Rocha-Singh et al.
2019/0321059	A1	10/2019	Takahashi et al.
2019/0336727	A1	11/2019	Yang et al.
2019/0357893	A1	11/2019	Weber
2020/0015966	A1	1/2020	Kiersey et al.
2020/0046944	A1	2/2020	Cottone
2020/0060718	A1	2/2020	Patel
2020/0078571	A1	3/2020	Kirt
2020/0129196	A1	4/2020	McCaffrey et al.
2020/0147347	A1	5/2020	Cottone
2020/0191279	A1	6/2020	John et al.
2020/0230357	A1	7/2020	Fitzgerald
2020/0246596	A1	8/2020	Panian
2020/0315639	A1	10/2020	Nicholson et al.
2020/0330111	A1	10/2020	Nicholson et al.
2020/0330731	A1	10/2020	Nicholson et al.
2020/0368496	A1	11/2020	Loesener et al.
2021/0045757	A1	2/2021	Bouasaysy
2021/0052321	A1	2/2021	Katoh et al.
2021/0085937	A1	3/2021	Dalvi
2021/0153882	A1	5/2021	Kugler et al.
2021/0162184	A1	6/2021	Lippert
2021/0338975	A1	11/2021	Cottone
2021/0346656	A1	11/2021	Lippert
2022/0211397	A1	7/2022	Nicholson et al.
2022/0280244	A1	9/2022	Zheng et al.
2023/0381452	A1	11/2023	Nishigishi

FOREIGN PATENT DOCUMENTS

DE	102018119605	A1	2/2020
JP	H10165508		6/1998
WO	WO 0134237	A1	5/2001
WO	WO 0170133	A2	9/2001
WO	WO 2006/046244		5/2006
WO	WO 2008024597	A2	2/2008

WO	WO 2009100129	A2	8/2009
WO	WO 2012068273	A1	5/2012
WO	WO 2012158152	A1	11/2012
WO	WO 2013003757	A2	1/2013
WO	WO 2017175531	A1	10/2017
WO	WO 2018/165277		9/2018
WO	WO 2019005903	A1	1/2019
WO	WO 2019/209798		10/2019
WO	WO 2020/076833		4/2020
WO	WO 2020/206101		10/2020
WO	WO 2021/014316		1/2021
WO	WO 2021021368	A1	2/2021
WO	WO 2021/084460		5/2021
WO	WO 2021/084462		5/2021
WO	WO 2021/086903		5/2021
WO	WO 2021163635	A1	8/2021

OTHER PUBLICATIONS

Final Office Action mailed Oct. 5, 2022, in U.S. Appl. No. 17/656,974.

European extended supplementary Search Report mailed Mar. 14, 2023, in EP Application No. 20784940.7.

European partial Search Report, lack of unity rejection, and search opinion mailed Dec. 9, 2022, in EP Application No. 20784940.7.

International Search Report for International Application No. PCT/US20/26360 dated Jun. 25, 2020.

Office Action mailed Apr. 13, 2022, in U.S. Appl. No. 16/838,841.

Response to Office Action filed Jul. 7, 2022, in U.S. Appl. No. 16/838,841.

Office Action mailed Jun. 8, 2022, in U.S. Appl. No. 17/656,974.

Office Action mailed Nov. 9, 2022, in U.S. Appl. No. 16/838,841.

Amendment After Final filed Jan. 9, 2023, in U.S. Appl. No. 16/838,841.

Office Action mailed Apr. 28, 2023, in U.S. Appl. No. 16/838,841.

Amendment After Final filed Oct. 19, 2022, in U.S. Appl. No. 17/656,974.

Notice of Allowance mailed Nov. 16, 2022, in U.S. Appl. No. 17/656,974.

Final Office Action mailed Oct. 31, 2023, in U.S. Appl. No. 16/838,841.

Amendment After Final filed Jan. 2, 2024, in U.S. Appl. No. 16/838,841.

Office Action mailed Feb. 27, 2024, in U.S. Appl. No. 16/838,841.

* cited by examiner

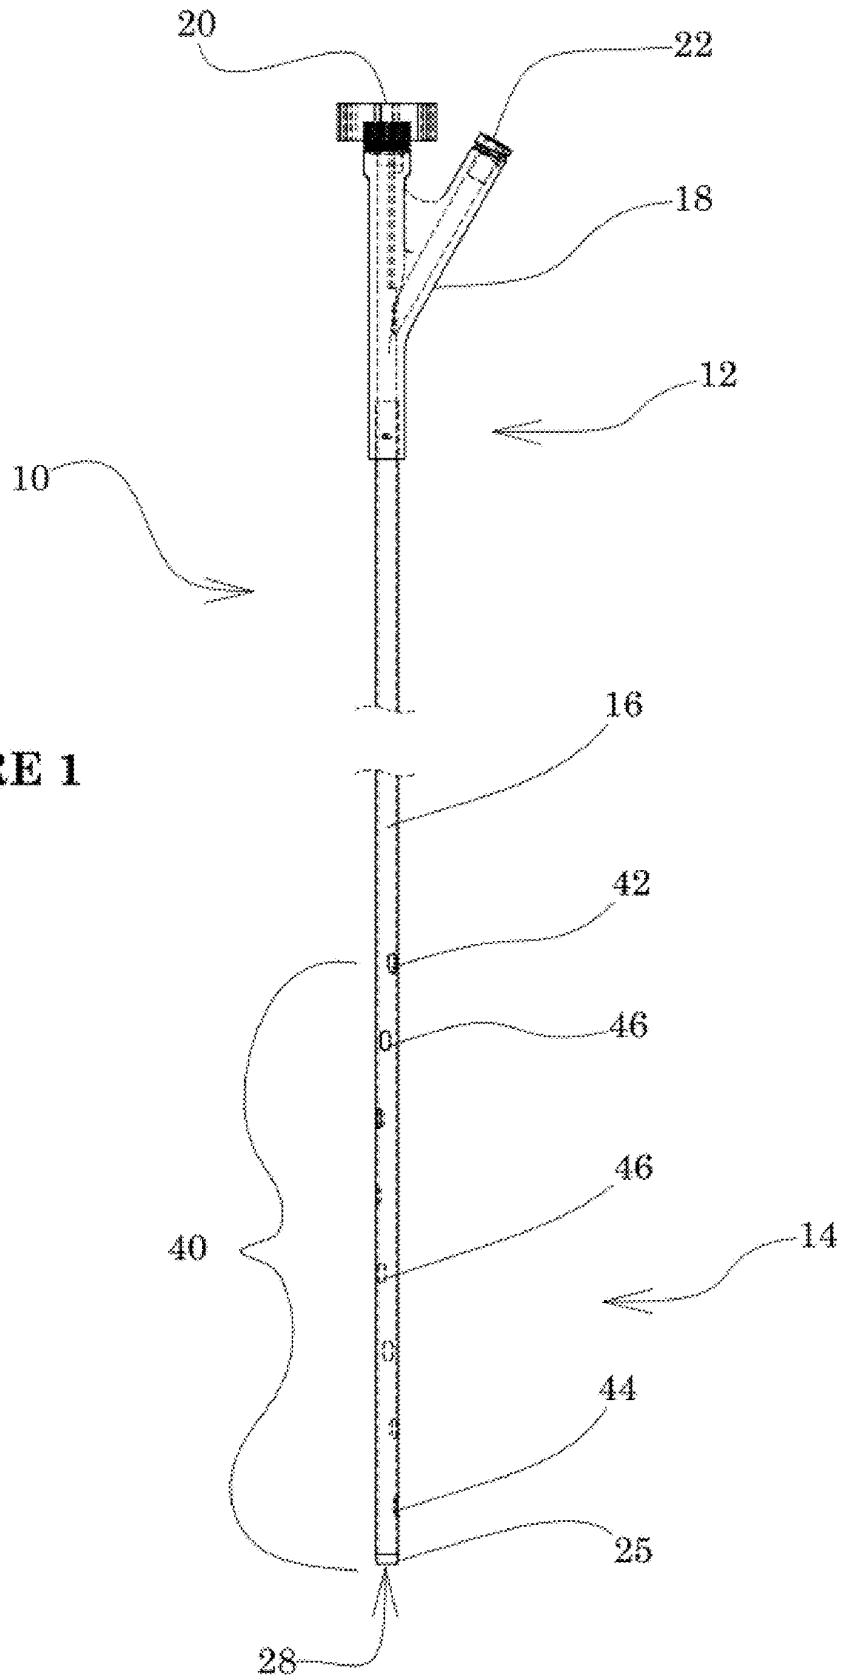


FIGURE 2

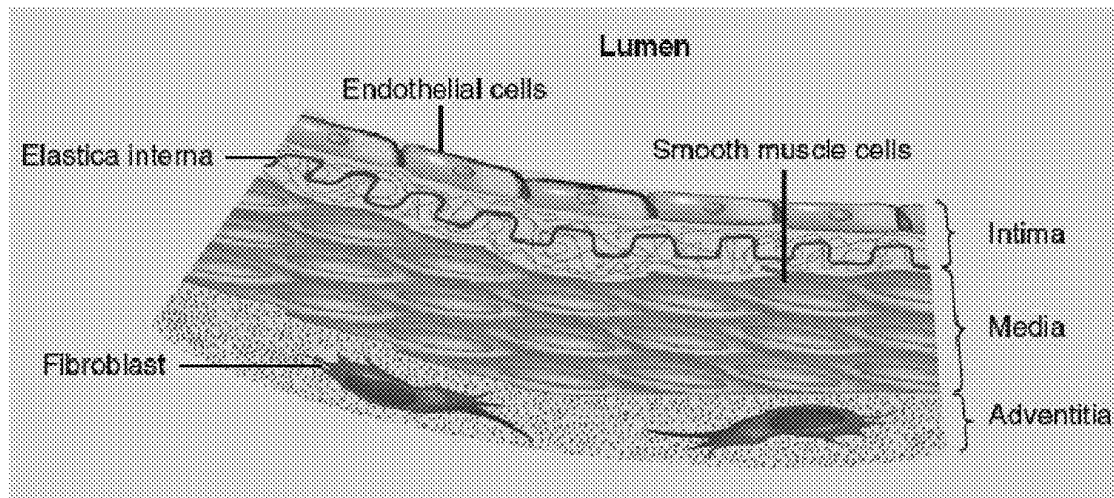


FIGURE 3A

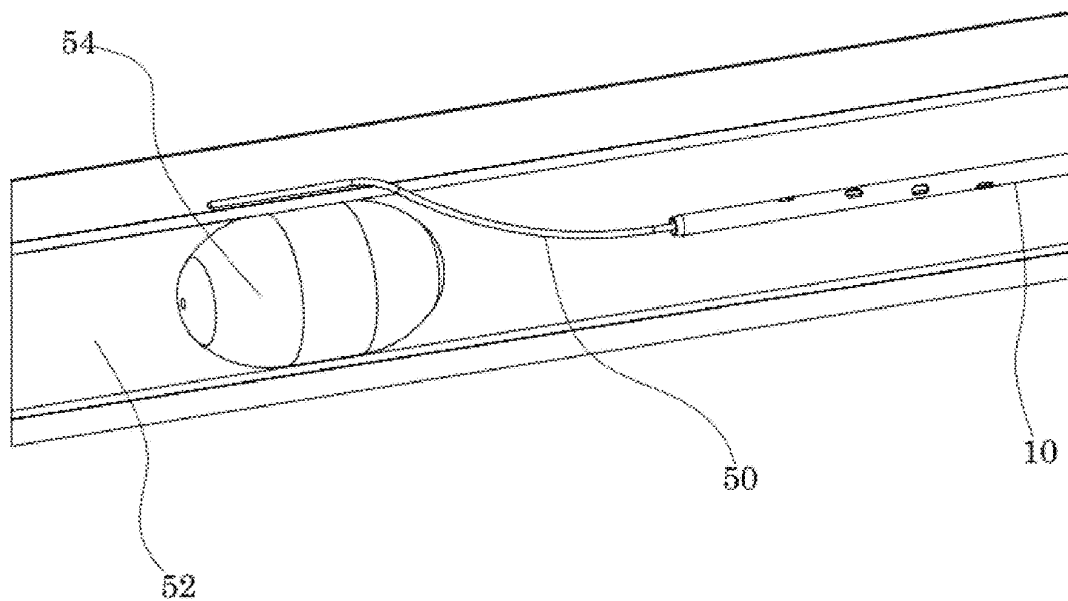


FIGURE 3B

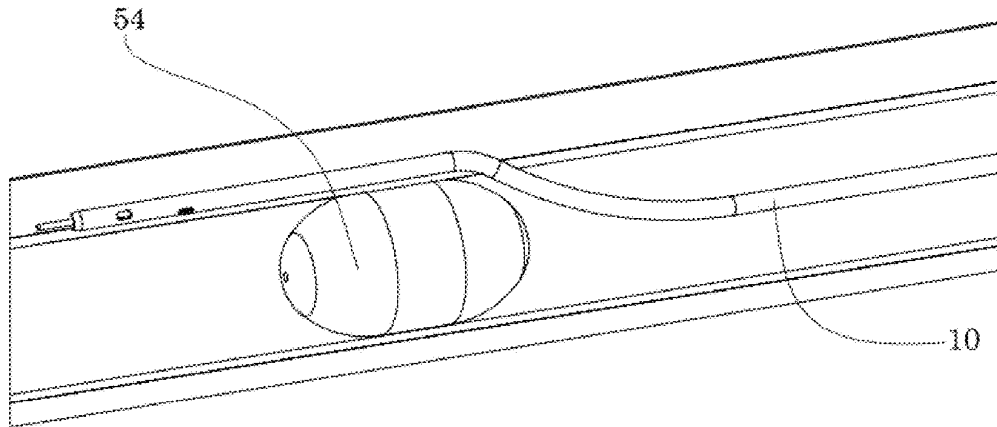


FIGURE 3C

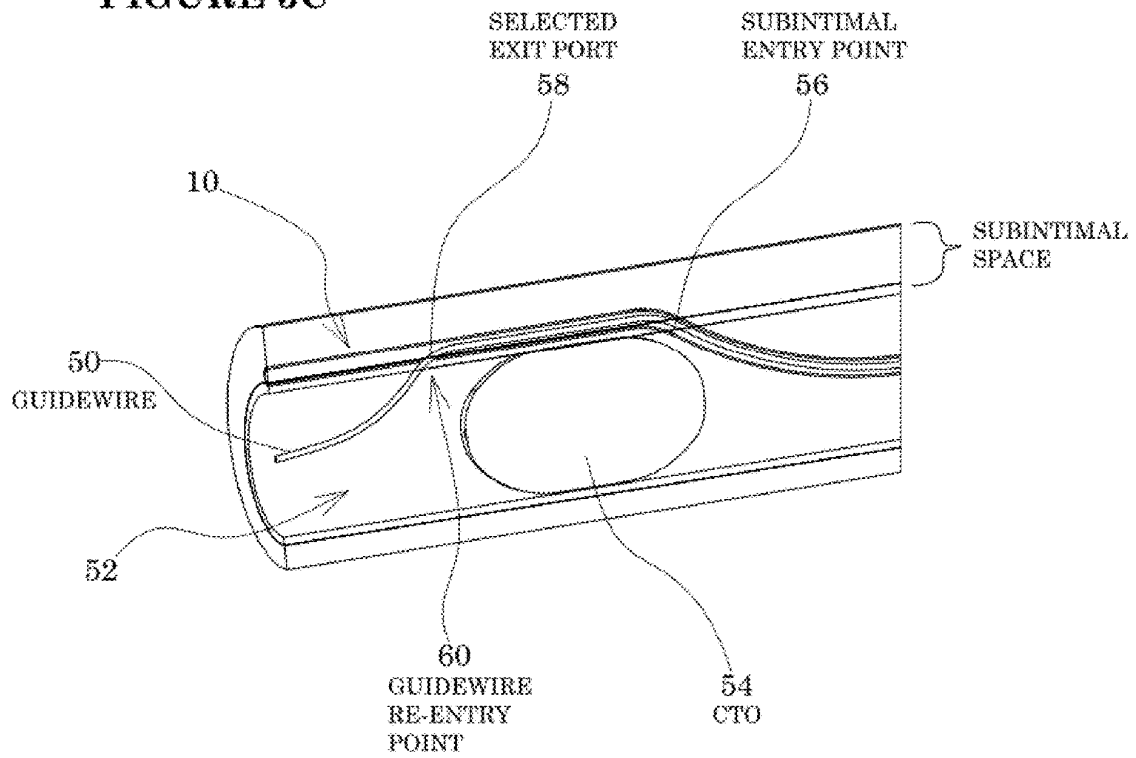


FIGURE 3D

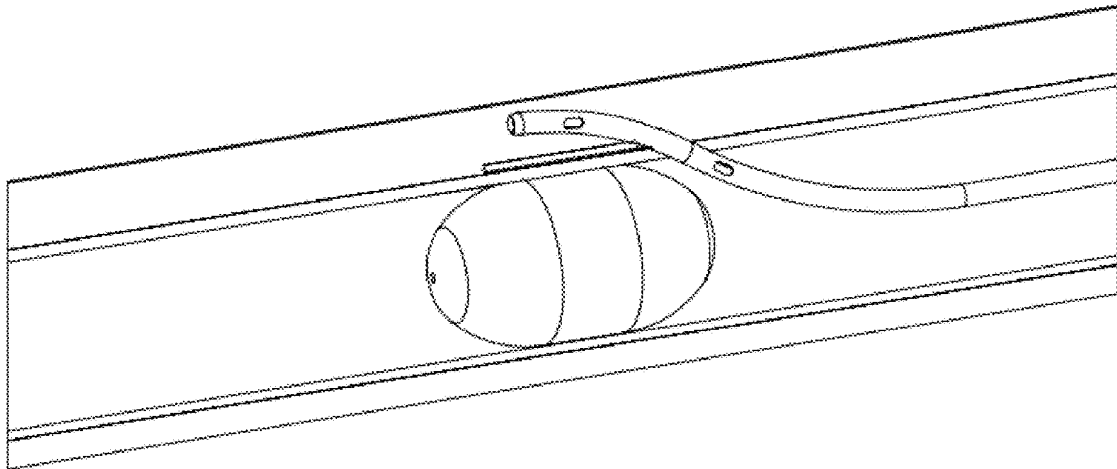


FIGURE 3E

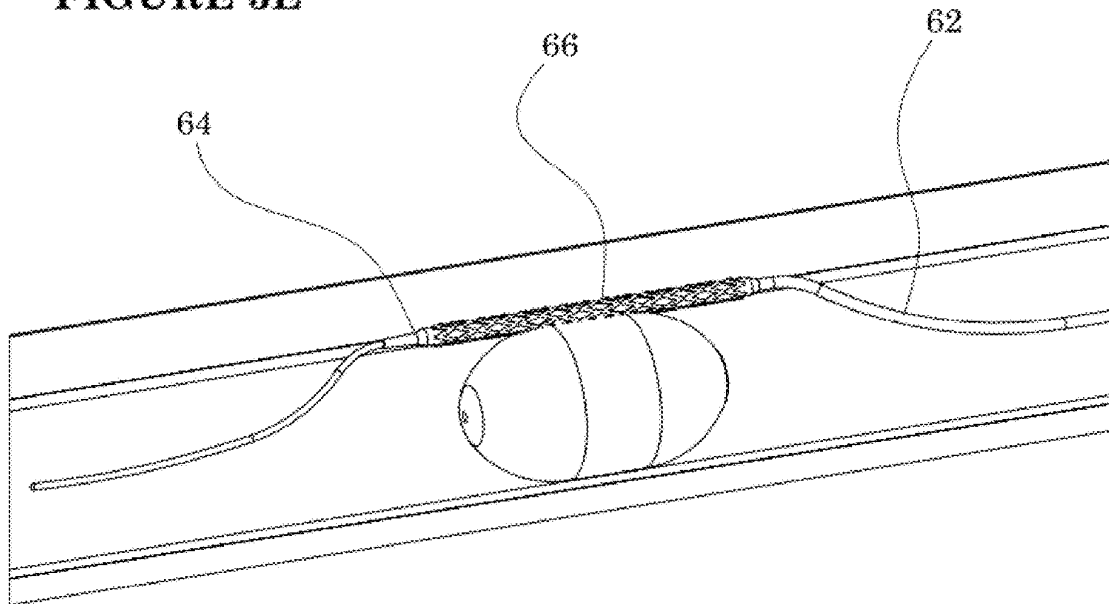


FIGURE 3F

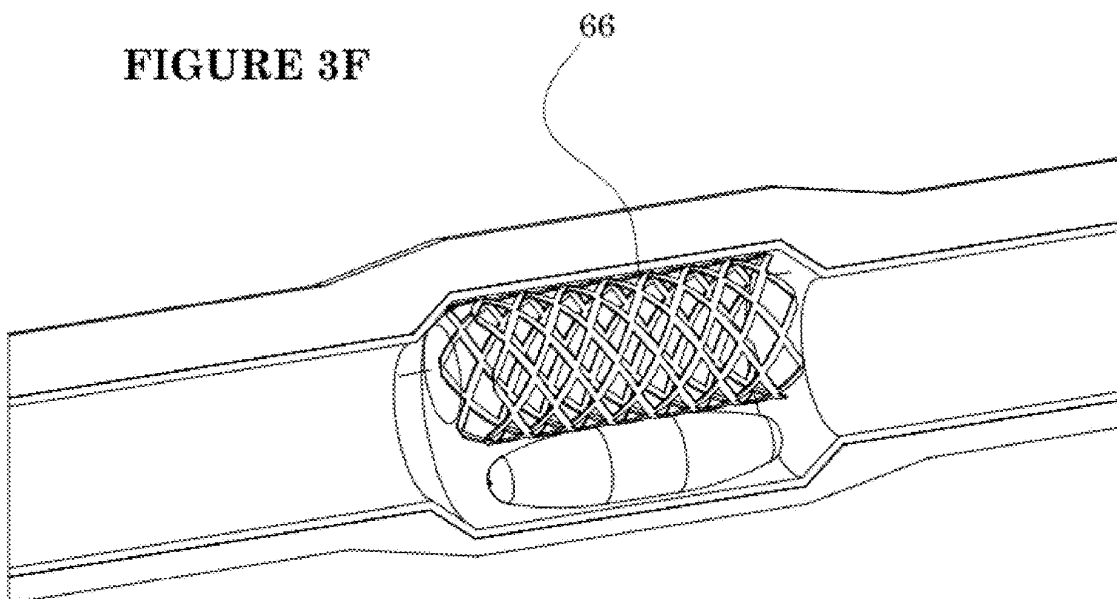


FIGURE 4A

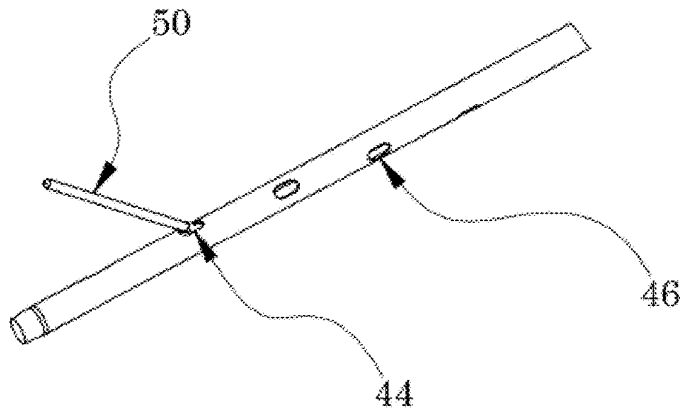


FIGURE 4B

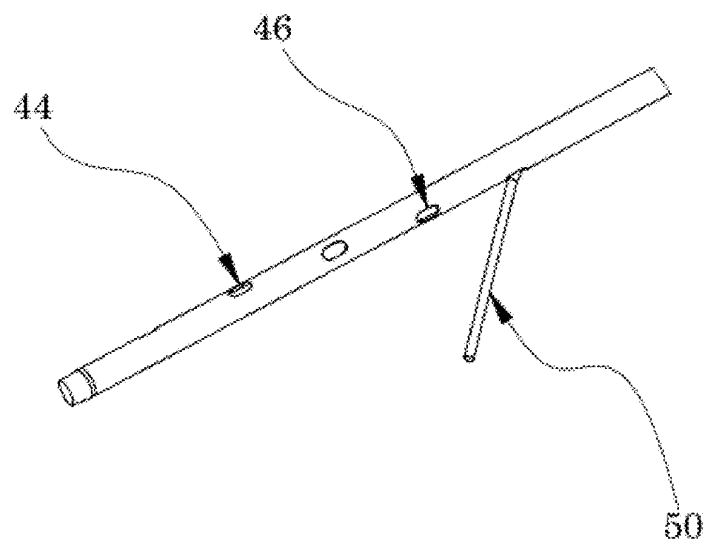


FIGURE 5A

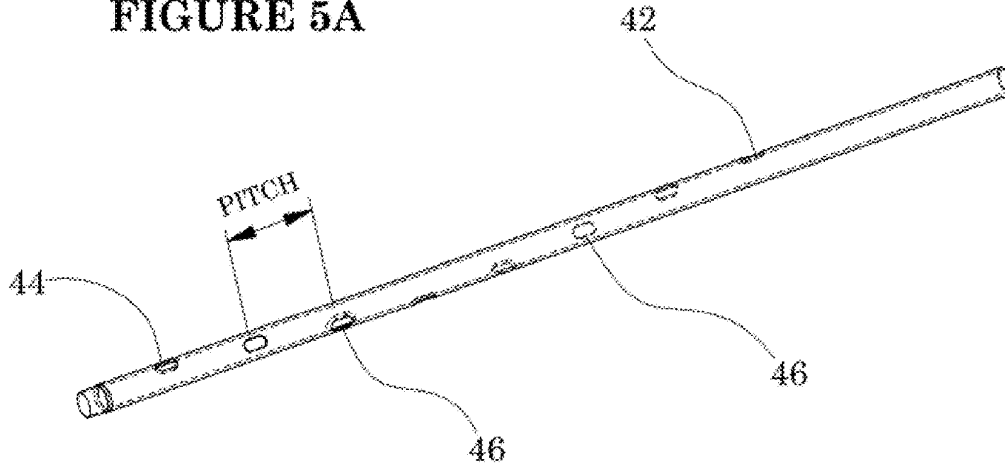


FIGURE 5B

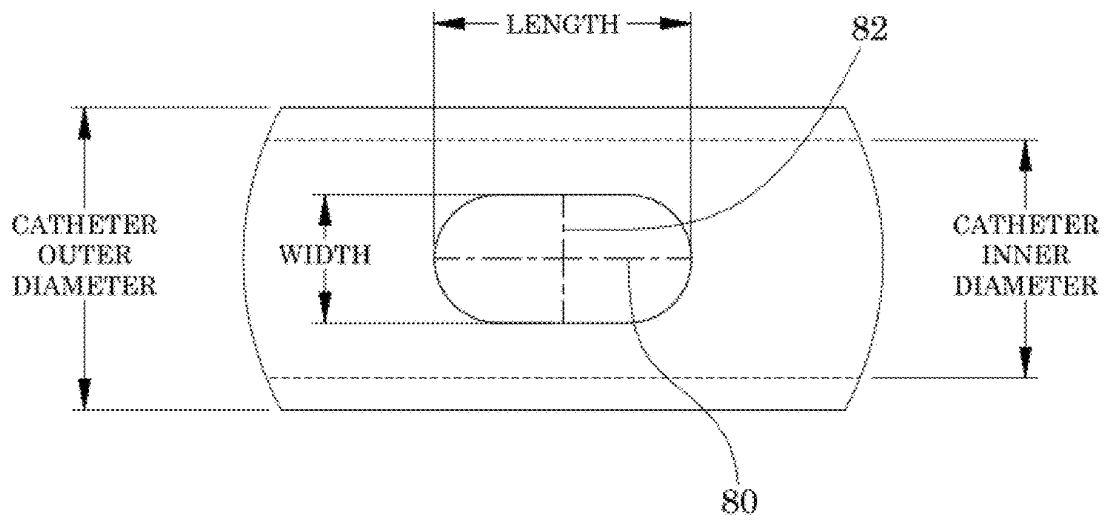


FIGURE 6A

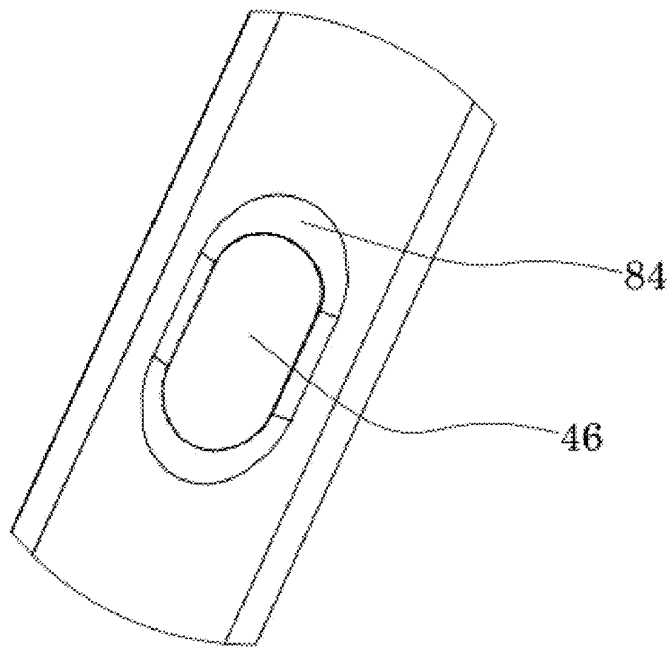


FIGURE 6B

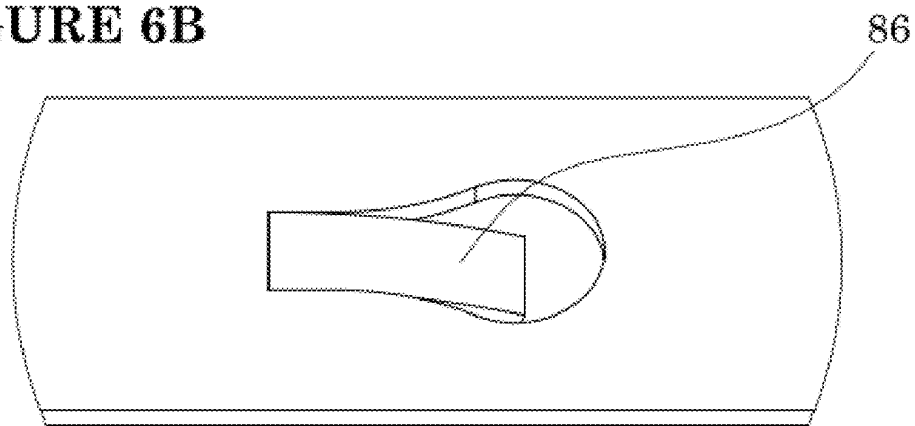


FIGURE 6C

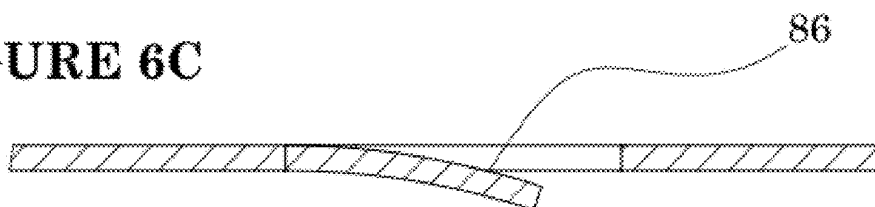


FIGURE 7A

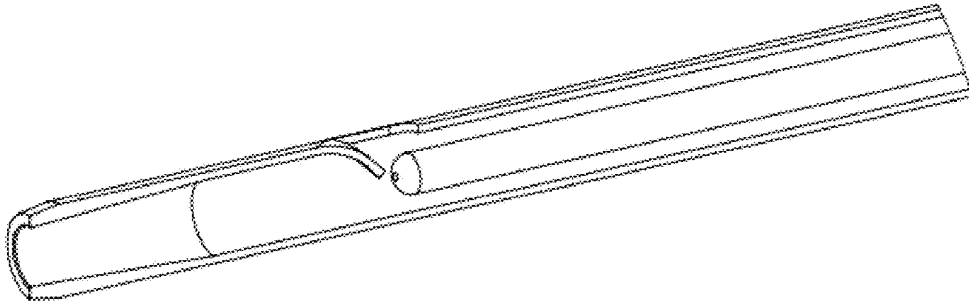


FIGURE 7B

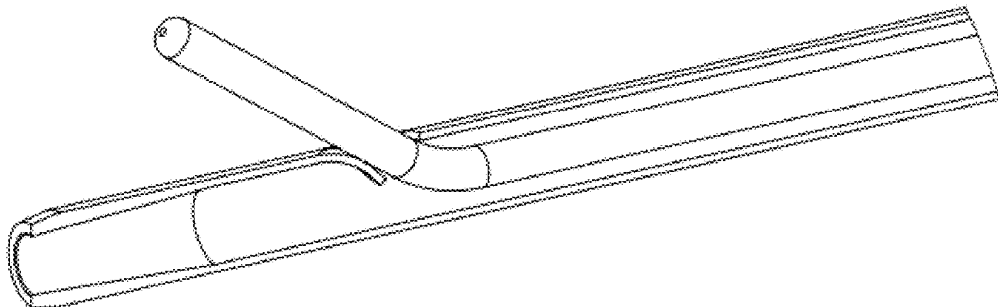


FIGURE 8

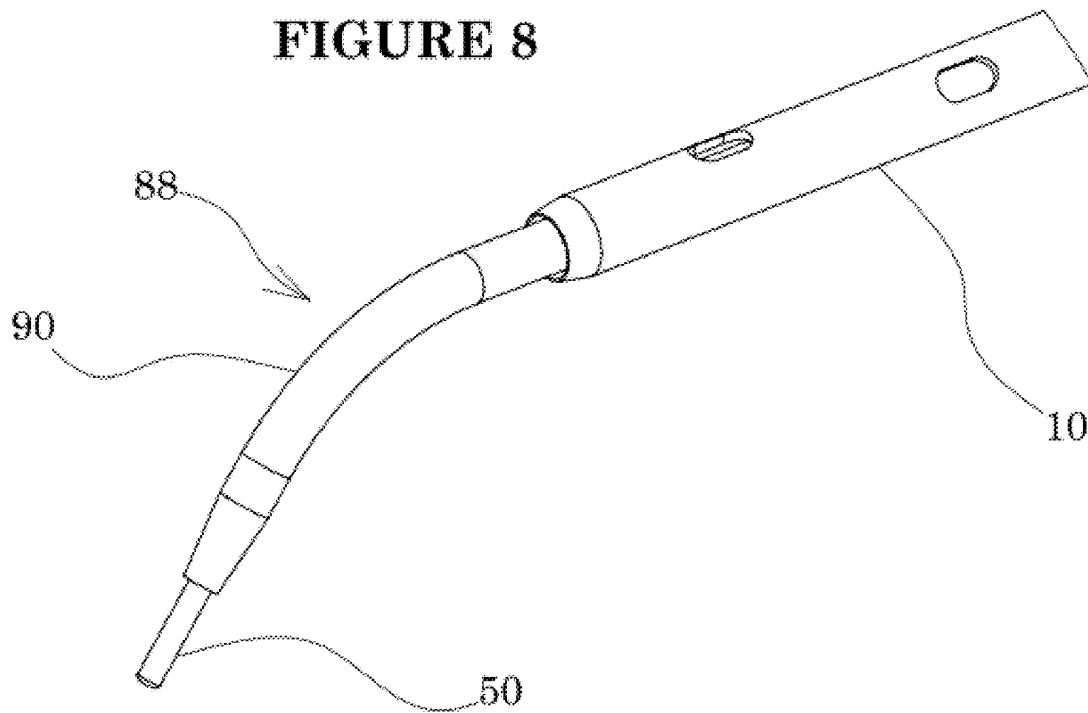


FIGURE 9

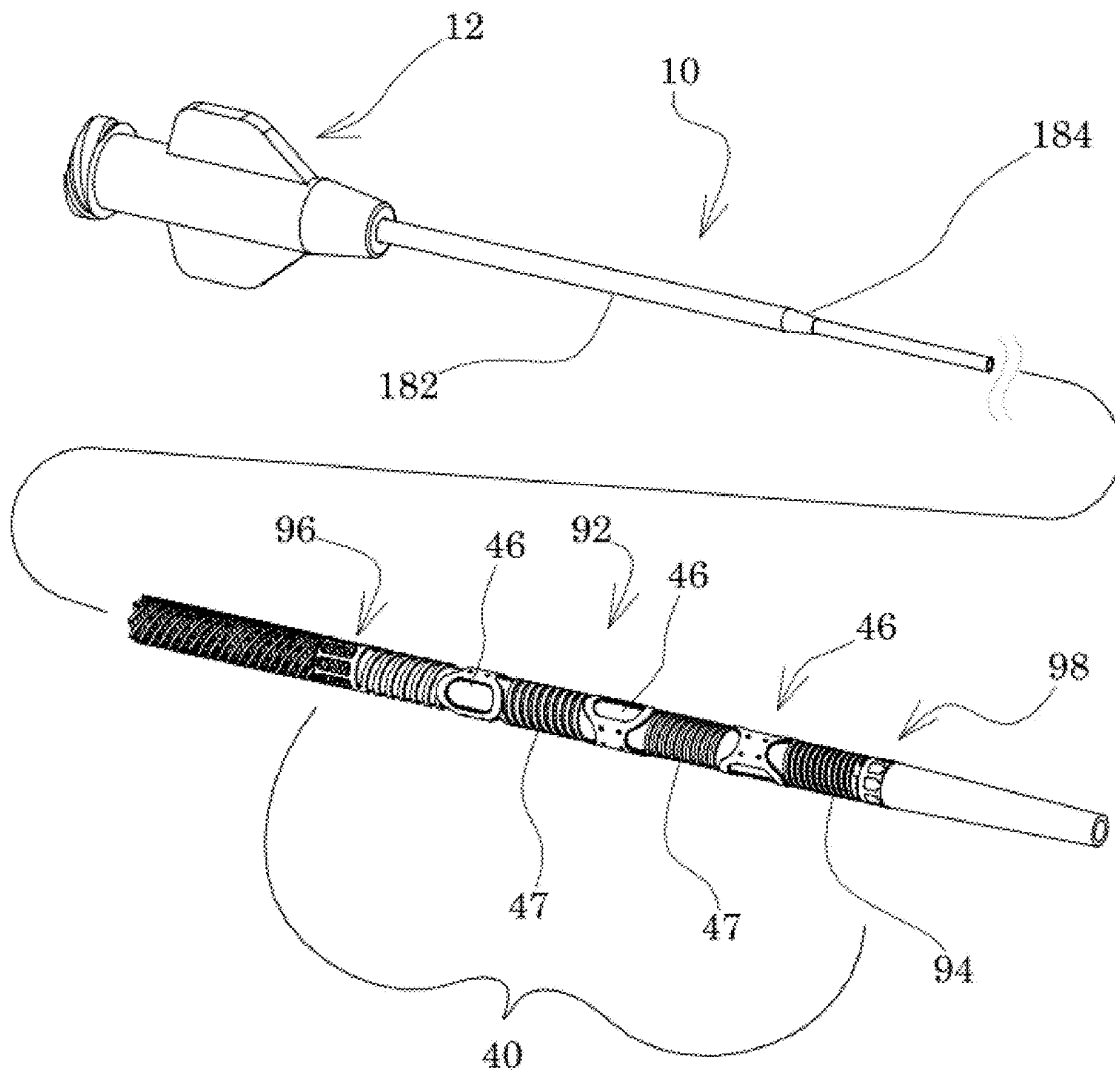


FIGURE 10A

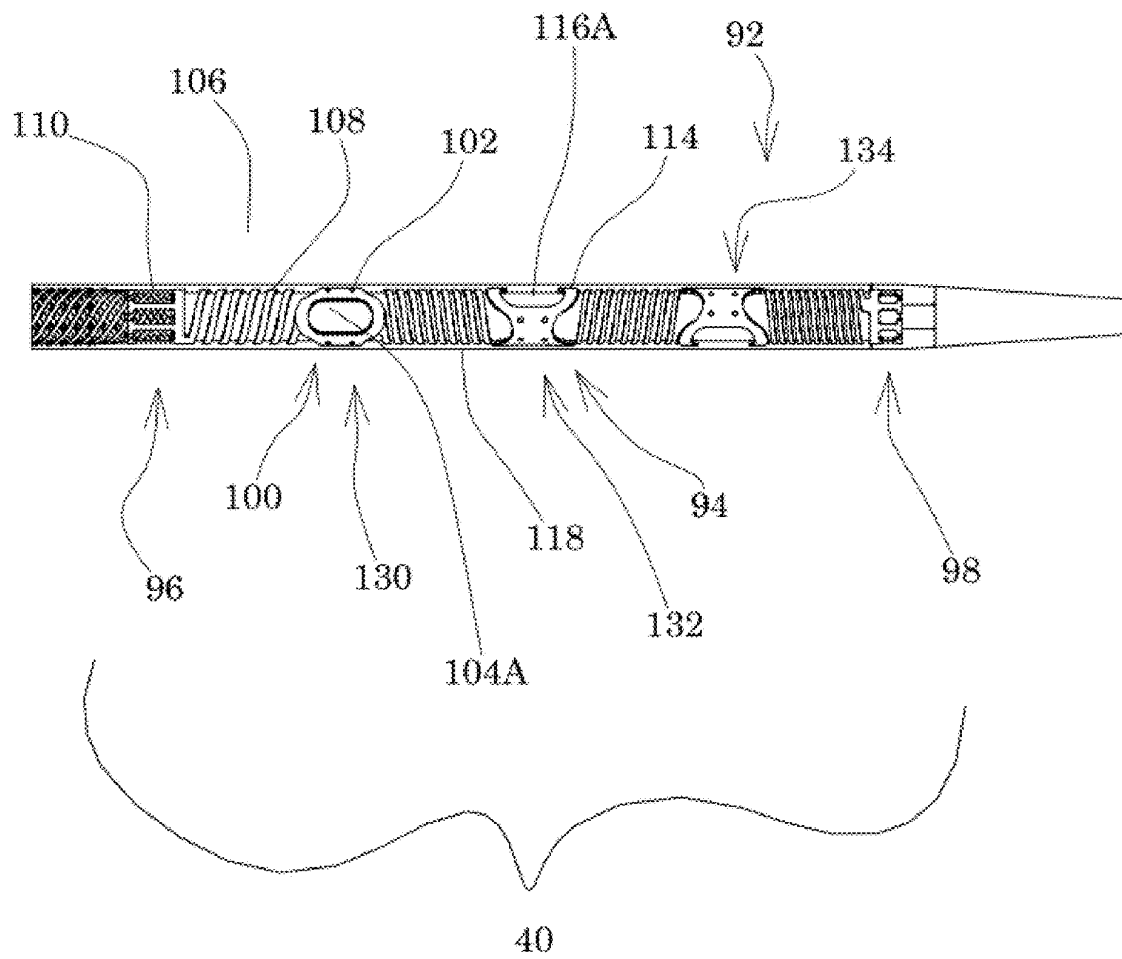


FIGURE 10B

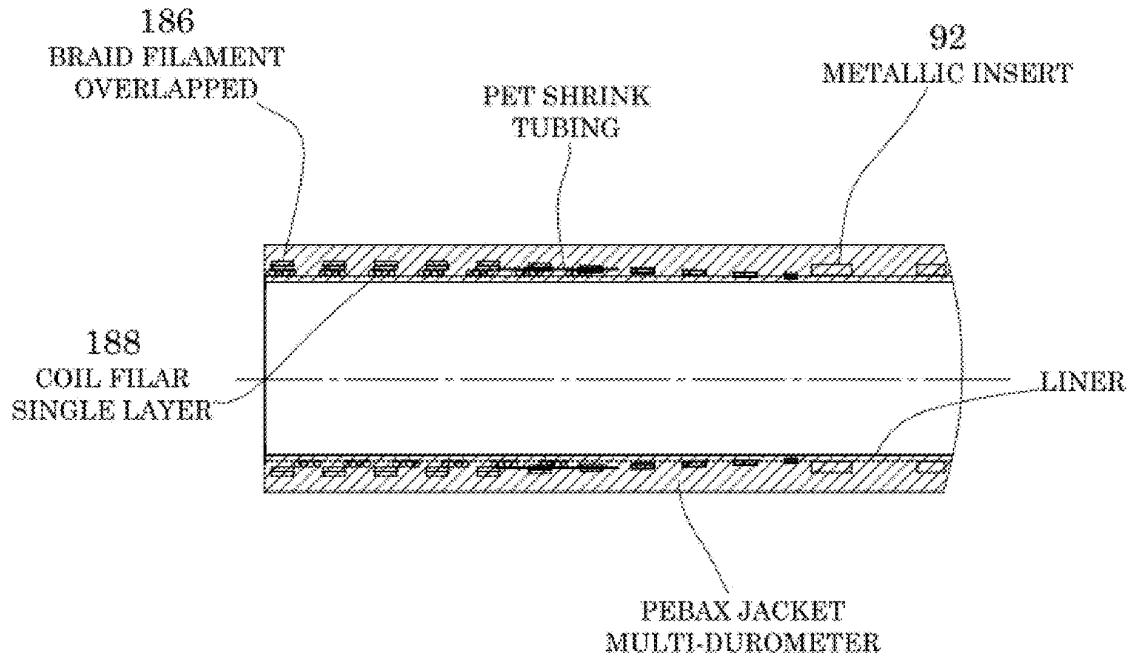


FIGURE 10C

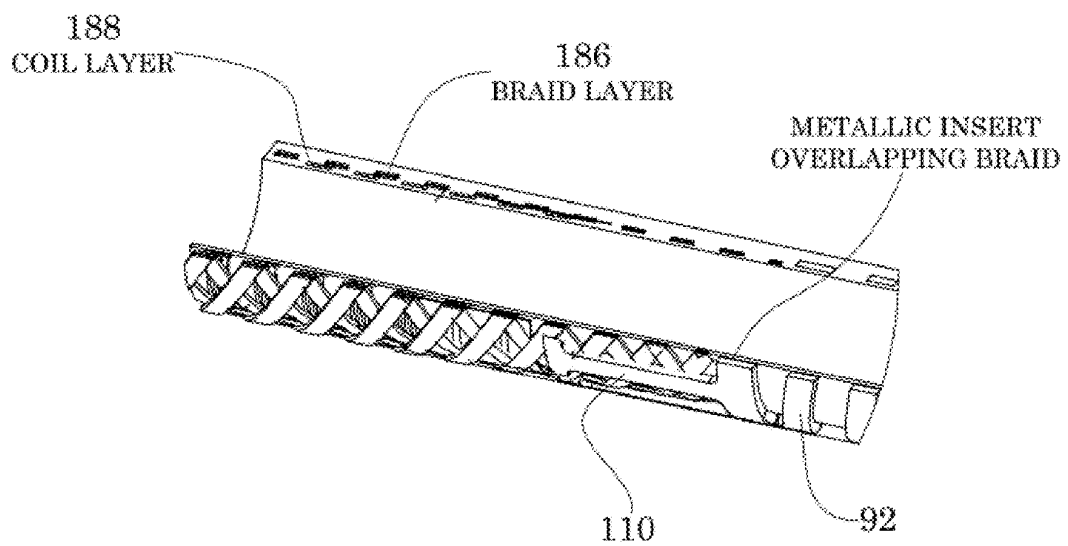


FIGURE 10D

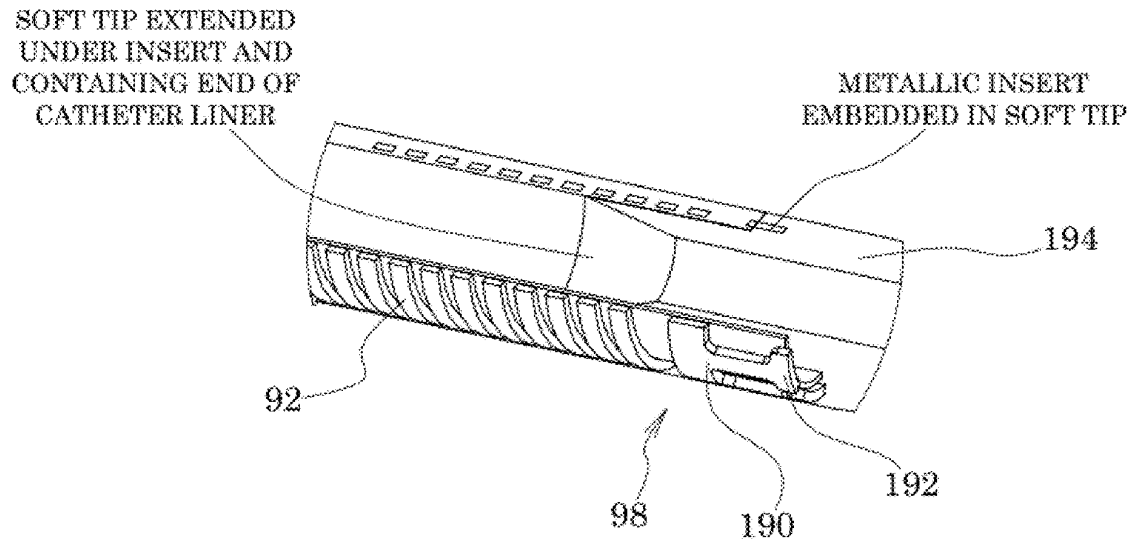


FIGURE 10E

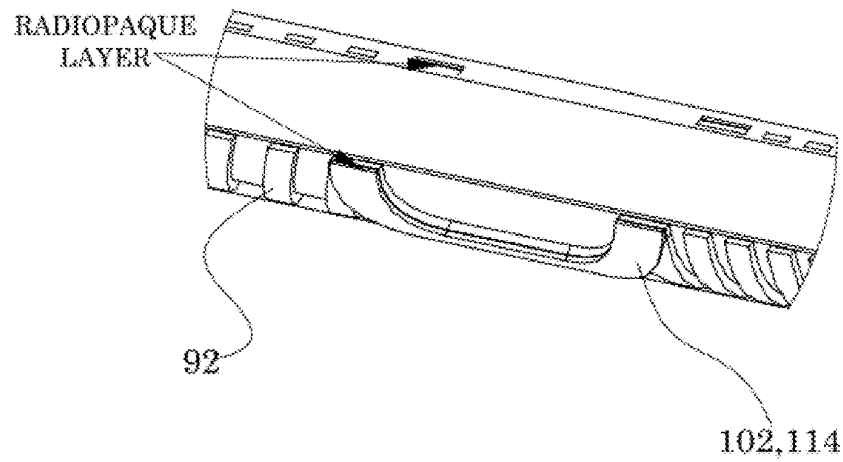


FIGURE 11A

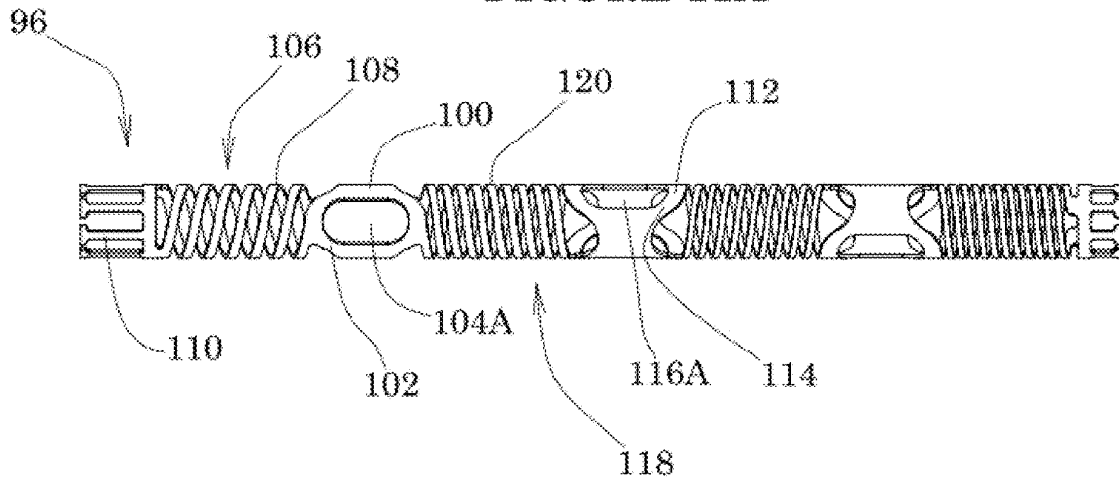


FIGURE 11B

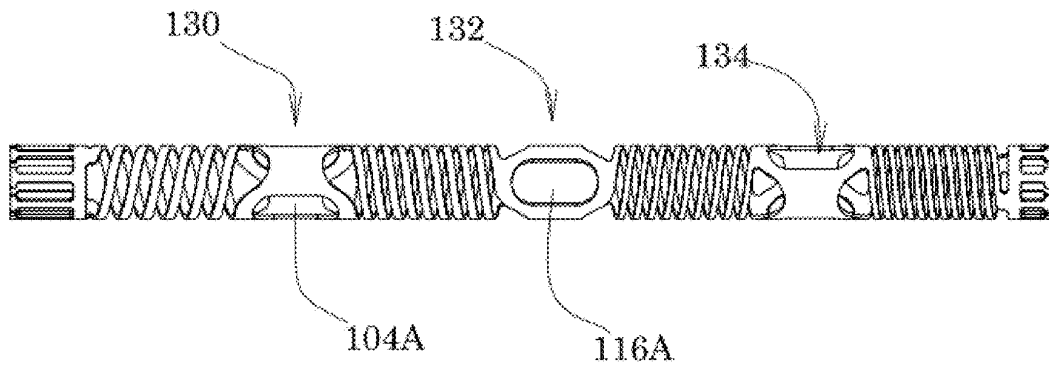


FIGURE 11C

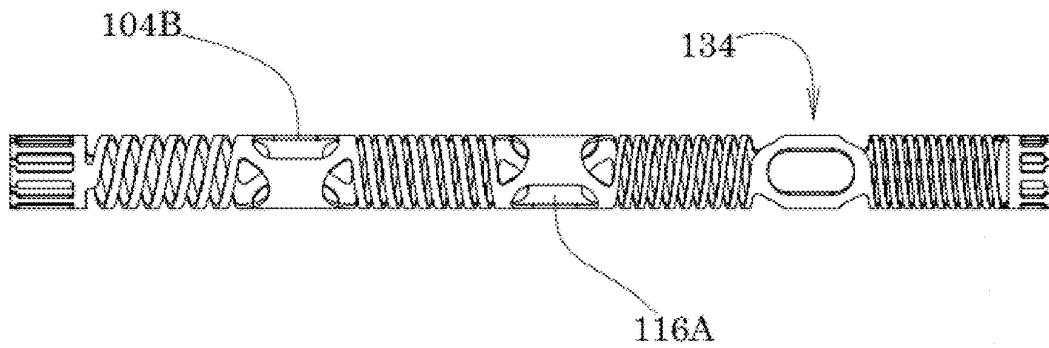


FIGURE 11D

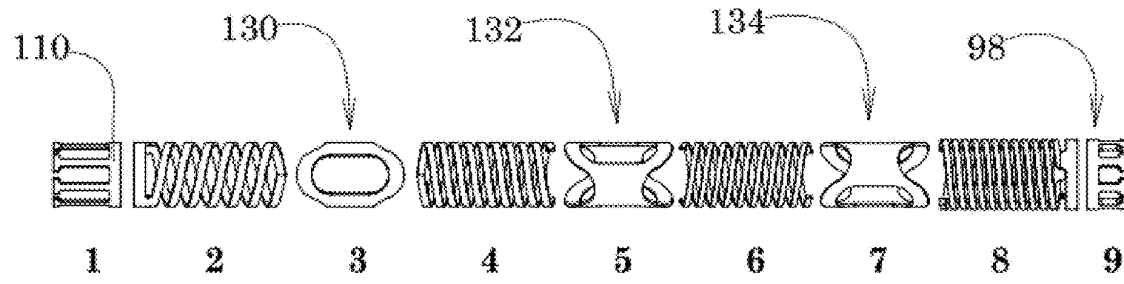


FIGURE 11E

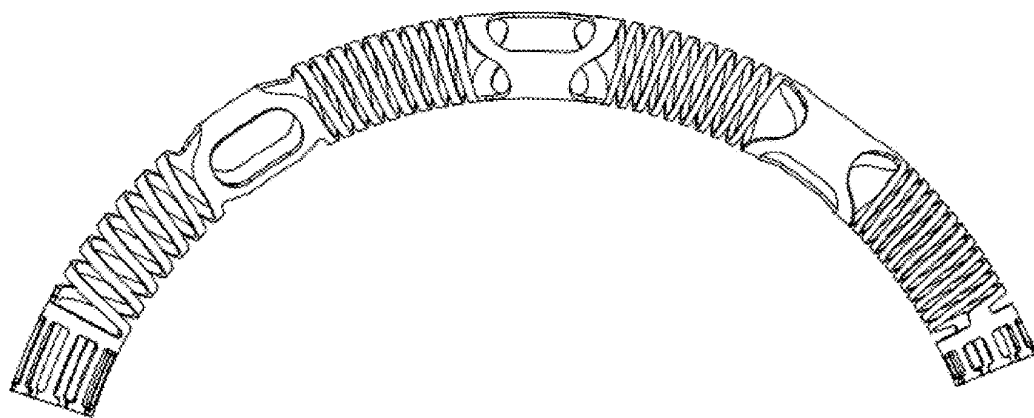


FIGURE 12

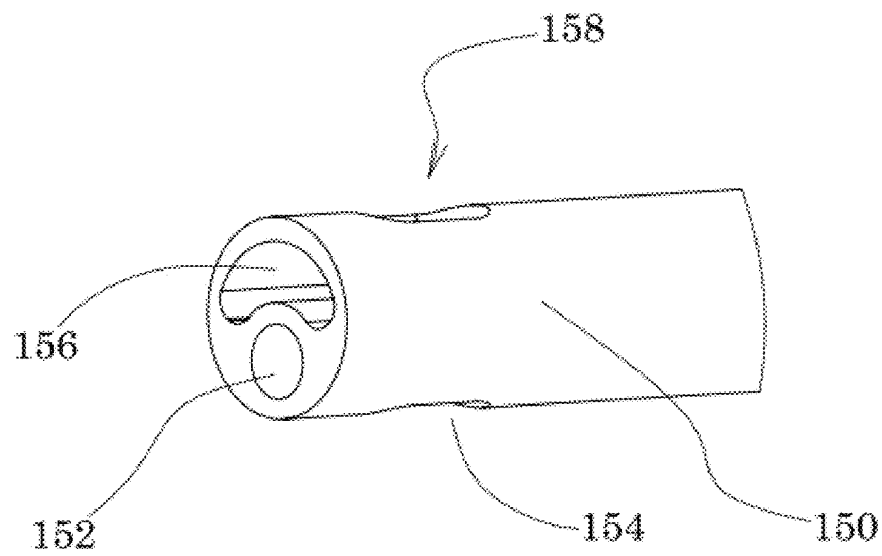


FIGURE 13



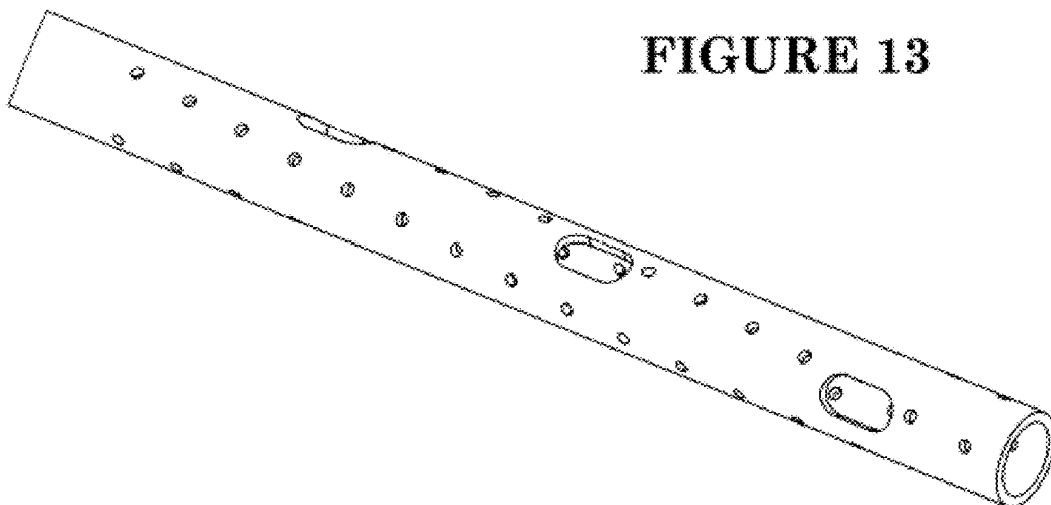


FIGURE 14

Visualization under Fluoroscopy

- The catheter tip and/or shaft may be made of RO material for enhanced visualization under fluoroscopy

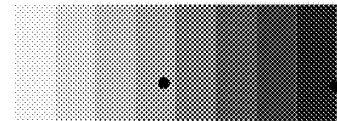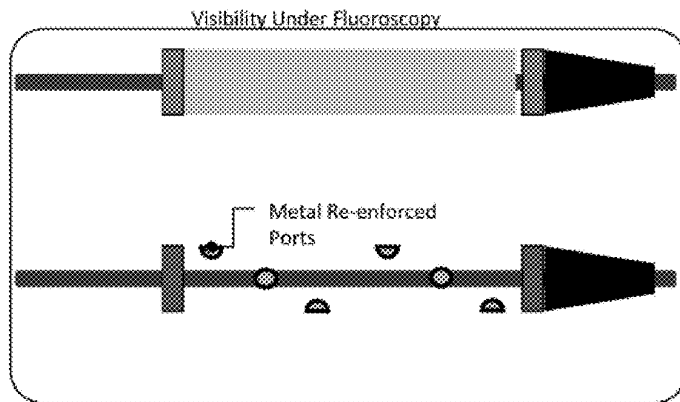

50%
RO

100%
RO

Configuration 1:

- Tapered Tip: 100% RO
- Guidewire: 80% RO
- Marker Bands: 60-70% RO
- Landing Zone: 50%

Configuration 2:

- Tapered Tip: 100% RO
- Guidewire: 80% RO
- Marker Bands: 60-70% RO
- Landing Zone: Radiolucent
- Ports: 50% Metal Re-enforced

FIGURE 15

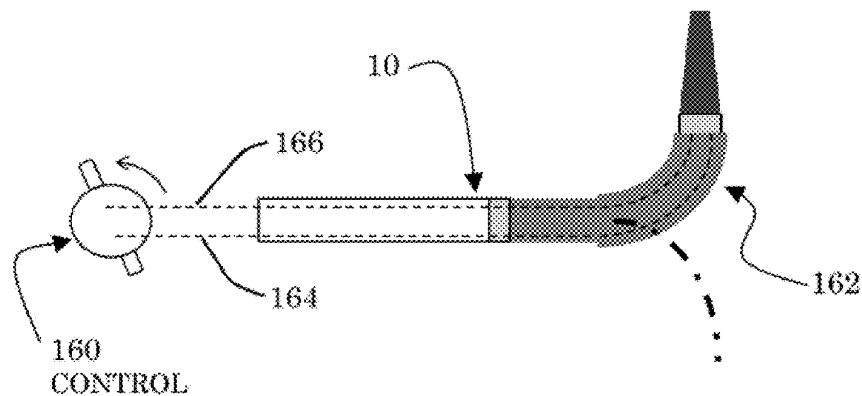


FIGURE 16

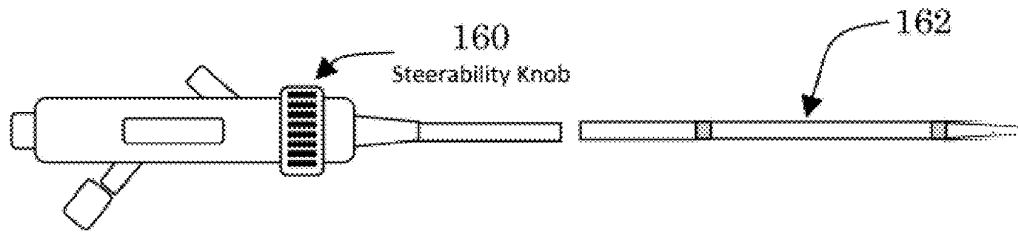


FIGURE 17

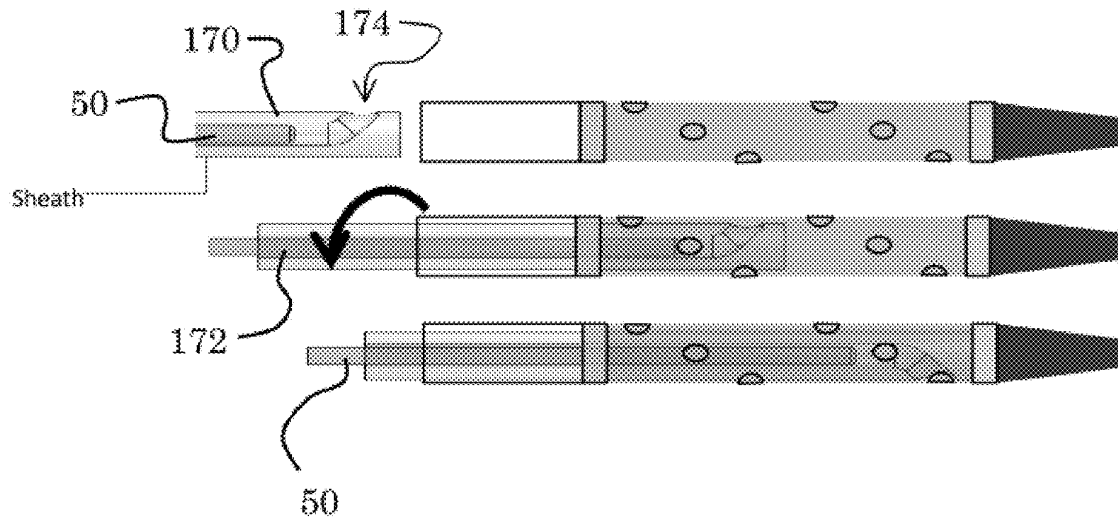


FIGURE 18

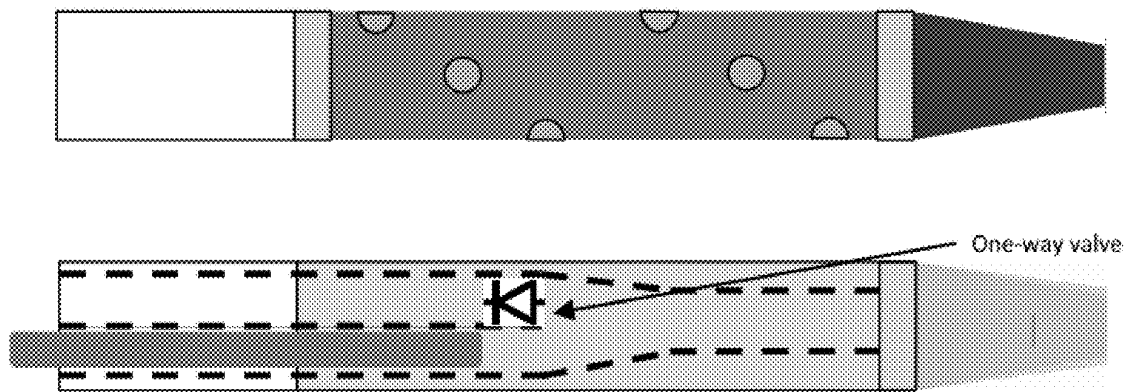


FIGURE 19


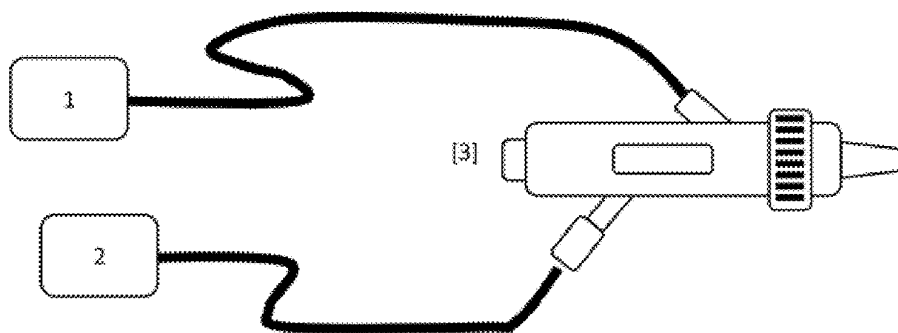


FIGURE 20

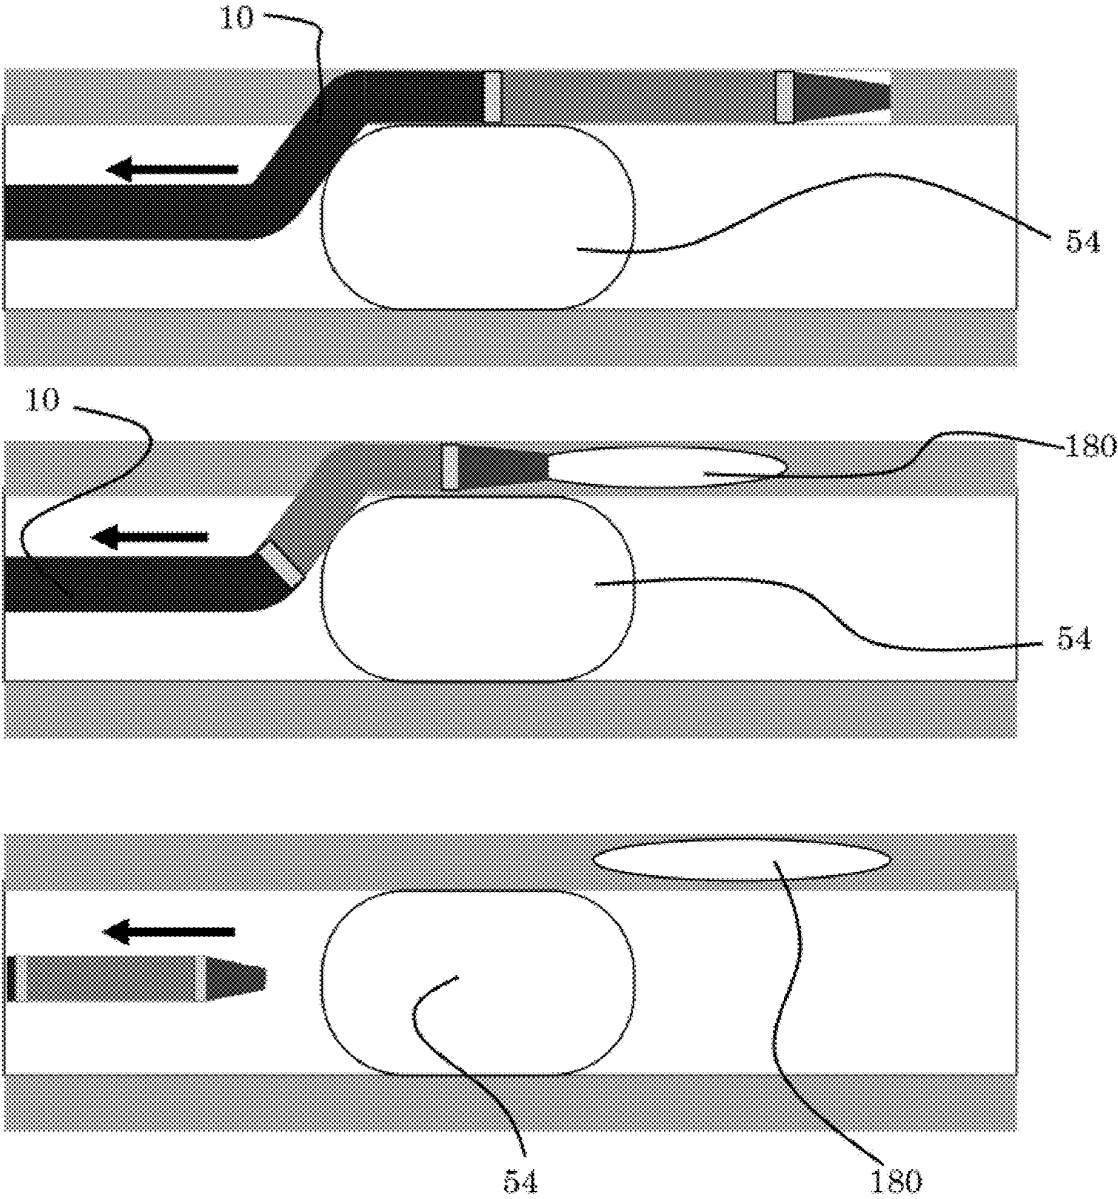

REENTRY CATHETER FOR CROSSING A VASCULAR OCCLUSION

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a continuation of U.S. application Ser. No. 16/838,863, filed Apr. 2, 2020, now U.S. Pat. No. 11,154,312, which claims priority to U.S. Provisional Patent Application No. 62/830,199, filed Apr. 5, 2019, and to U.S. Provisional Patent Application No. 62/907,299, filed Sep. 27, 2019, the entire contents of each of which are incorporated herein by reference in their entireties.

BACKGROUND OF THE INVENTION

An interventional guide wire or other interventional device is often used in medical procedures that attempt to establish a pathway through a heavily stenosed or chronically occluded vessel. A chronically occluded vessel is referred to as containing a chronic total occlusion or CTO. During these procedures, the guide wire or device can only be of clinical benefit to establish vessel patency if it is advanced distally into the vessel true lumen.

One technique for restoring patency across a CTO involves advancing a guide wire through the intimal layer of the vessel wall and into the subintimal plane or space, where it can be further advanced distally beyond the CTO. Once in this sub-intimal plane beyond the CTO, it becomes difficult to navigate the guide wire or device back through the subintimal tissue layer to re-gain access into the vessel true lumen, sometimes referred to as a "reentry" into the vessel lumen from the sub-intimal space distally of the CTO. The layer of tissue that separates the vessel true lumen from the subintimal plane is typically in the range from 100 to 500 micrometers thick for vessels in the diameter range from 2 mm to 4 mm, and from 100 to 3000 microns thick, in the largest vessels of the body.

A variety of catheters have been proposed for reentry around a CTO. One is described and shown in U.S. Pat. No. 6,231,546. In this system, the re-entry catheter requires the operator to rotate a catheter shaft while observing a radiopaque marker on the catheter shaft to ensure that a side or lateral port is aimed at the true lumen of the blood vessel. Once the marker indicates the correct orientation of the lateral port, a cannula is extended through the lateral port in order to penetrate through the intimal layer of the blood vessel. It is believed that one drawback of this system is the requirement to rotate the catheter to the correct position while under fluoroscopic imaging otherwise an incorrect orientation of the cannula could cause failure to reenter the parent lumen and potentially cause damage to the vessel.

Another system is described and illustrated in US Patent Application Publication 2013/0072957. In this publication, a balloon is used to orient the cannula into the proper orientation for re-entry into the true vessel lumen. To achieve this, the catheter utilizes an asymmetrical catheter lumen for the cannula. It is believed that this system also suffers from a similar drawback in that the lateral port of the cannula must be oriented in the correct direction towards the true lumen while under fluoroscopy. This is to ensure that the cannula does not penetrate away from the true lumen, which could lead to internal hemorrhaging.

Despite the foregoing and other efforts in the prior art, there remains a need for an improved reentry catheter and method for traversing total chronic occlusions.

SUMMARY OF THE INVENTION

Disclosed is a reentry catheter for crossing a vascular occlusion. The catheter includes an elongate flexible tubular body, having a proximal end, a distal end and at least one lumen extending there through. A reentry zone on the tubular body includes at least two and preferably at least three or five or more exit apertures in communication with the lumen, the apertures rotationally offset from each other by at least about 15 degrees and aligned in a spiral pattern around the tubular body. In one implementation, three pairs of opposing apertures are provided.

A method of crossing a chronic total occlusion includes the steps of advancing a guidewire from a vascular lumen through the intima, into a subintimal space and distally beyond the occlusion. A reentry catheter is advanced over the guidewire and beyond the occlusion, such that at least one of a plurality of spirally aligned exit ports on the reentry catheter is rotationally aligned with the lumen. The guidewire is advanced through the at least one exit port to cross the intima and reenter the lumen. The reentry catheter may be removed, and a balloon catheter may be advanced over the wire and the balloon expanded in the subintimal space to create a neolumen that permits perfusion across the occlusion. A stent may be expanded in the neolumen to maintain patency across the occlusion.

There is provided, in accordance with another aspect of the present invention, a re-entry catheter for crossing a vascular occlusion. The catheter comprises an elongate flexible tubular body, having a proximal end, a distal end and at least one lumen extending there through. A reentry zone is defined on the tubular body, comprising at least two exit apertures in communication with the lumen, the apertures rotationally offset from each other by at least about 5 degrees, and the reentry zone is positioned within about 20 cm of the distal end of the tubular body.

The re-entry zone may be comprised of at least three apertures, or at least five apertures, arranged in a spiral configuration around the tubular body. At least one aperture may have a noncircular configuration and at least one aperture may have a major axis in parallel to a longitudinal axis of the tubular body, and a minor, transverse axis. At least one aperture has a minor axis diameter of at least about 0.025 mm.

In accordance with another aspect of the present invention, there is provided a method of crossing a chronic total occlusion. The method comprises the steps of advancing a guidewire from a vascular lumen through the intima, into a subintimal space and distally beyond the occlusion. A reentry catheter is advanced over the guidewire and beyond the occlusion, such that at least one of a plurality of exit ports on the reentry catheter is rotationally aligned with the lumen. The guidewire is advanced through the at least one exit port to cross the intima and reenter the lumen.

The method may additionally comprise the step of applying vacuum to the central lumen or secondary lumen to draw adjacent tissue against one or more side ports. Vacuum may also be used to aspirate hematoma or other embolic material into one or more side ports, and/or the distal guidewire opening into the central lumen.

The method may further comprise the step of proximally retracting the catheter, leaving the guidewire extending into the lumen distally of the occlusion. A balloon catheter may be advanced over the wire and the balloon expanded in the subintimal space. A stent may be expanded in the subintimal space to maintain patency of a neolumen that permits perfusion across the occlusion.

3

In accordance with a further aspect of the present invention, there is provided a reentry catheter for crossing a vascular occlusion, comprising an elongate flexible tubular body, having a proximal end, a distal end and at least one lumen extending there through; and a reentry zone on the tubular body, comprising at least three opposing pairs of side wall exit apertures in communication with the lumen, each opposing pair of apertures rotationally offset from an adjacent opposing pair of apertures.

The reentry catheter may additionally comprise a reinforcing ring surrounding each aperture. The catheter may be provided with six reinforcing rings, one for each aperture, and the reinforcing rings may be connected together by a frame in the side wall which may be in the form of a tubular support. The reinforcing rings may comprise a radiopaque material. The frame may comprise a helical strut extending between a first and second axially spaced apart opposing pairs of side wall exit apertures.

The catheter may further comprise an inflatable balloon on the tubular body, in communication with a second, inflation lumen extending axially through the tubular body. A guidewire lumen may extend axially through the tubular body between a proximal port and a distal port, and the proximal port may be spaced distally apart from the proximal end or at the proximal end of the tubular body. The proximal port is within about 20 cm of the distal end of the tubular body.

There is also provided an intravascular catheter with fluoroscopically visible indicium of rotational orientation. The catheter comprises an elongate flexible tubular body, having a proximal end, a distal end and a tubular side wall defining at least one lumen extending there through; and first and second opposing pairs of radiopaque rings in the side wall, spaced axially apart from each other; wherein a first transverse axis extending through the first pair of rings is rotationally offset from a second transverse axis extending through the second pair of rings.

The intravascular catheter may further comprise an aperture in the side wall through each ring. The catheter may further comprise a frame connecting the rings, which may comprise one or more struts configured to provide a flexible hinge. At least a portion of the frame in between the first and second opposing pairs of rings in one implementation comprises a spring hinge in the form of at least one helical strut.

In accordance with a further aspect of the present invention, there is provided a subassembly for integration into the wall of a catheter. The subassembly comprises a tubular body having a plurality of aperture portions and intervening hinge portions. Each aperture portion includes a first and a second aperture carried on opposing sides of the tubular body. A first axis extending transversely through the tubular body and the first and second apertures of a first aperture portion is rotationally offset from a second axis extending transversely through the tubular body and the first and second apertures of a second aperture portion.

The hinge portion may comprise a helical strut. The aperture portions and intervening hinge portions may be parts of a unitary body which may be laser cut from a tube. Each aperture may be formed within an eyelet separated from an adjacent eyelet by a hinge portion.

An aperture may have a minor axis and a transverse major axis having a length of at least about 150% of the length of the minor axis. The subassembly body may have a wall thickness of no more than about 0.05 inches, and in some implementations no more than about 0.004 inches.

The subassembly may have at least three pairs of opposing apertures with intervening hinge portions between each

4

aperture pair. A first hinge portion may comprise a helical strut having a first pitch and a second hinge portion spaced apart from the first hinge portion by an aperture pair portion, may have a helical strut having a second, different pitch.

Further features and advantages of the invention will become apparent to those of skill in the art from the following description taken together with the associated drawings and claims.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a side elevational view of a reentry catheter in accordance with the present invention.

FIG. 2 shows the anatomy of a coronary artery.

FIG. 3A shows a guidewire entering a subintimal space to cross an occlusion.

FIG. 3B shows a reentry catheter tracking over the guidewire and through the subintimal space.

FIG. 3C shows the guidewire passing out of a selected exit port and back through the intima and into the true lumen distal to the occlusion.

FIG. 3D shows proximal retraction of the reentry catheter while leaving the guidewire in position across the occlusion.

FIG. 3E shows a balloon catheter carrying a balloon expandable stent positioned across the occlusion via the subintimal space.

FIG. 3F shows the catheter removed, leaving the stent expanded to support a neo lumen to permit perfusion across the occlusion in the native lumen.

FIG. 4A shows a reentry catheter with a guidewire exiting a first exit port at a first rotational orientation.

FIG. 4B shows a reentry catheter with a guidewire exiting a second exit port at a second rotational orientation.

FIGS. 5A and 5B show geometric aspects of the exit ports.

FIGS. 6A-6C show various exit port details.

FIGS. 7A-7B show lateral exit of a guide wire through an exit port with an exit ramp.

FIG. 8 shows a biased deflection guide for directing a guidewire toward the native lumen.

FIG. 9 shows a reentry catheter with a reinforced reentry zone.

FIG. 10A is a side elevational view of a reinforcing insert for supporting the reentry zone.

FIG. 10B is a side elevational cross section through the catheter wall at the transition between the braid and the proximal end of the reentry zone support.

FIG. 10C is a perspective view of the cross section shown in FIG. 10B.

FIG. 10D is a perspective cross sectional view of the transition between the distal end of the reentry support and the catheter tip.

FIG. 10E is a perspective cross sectional view of an eyelet formed by the reentry support, having a radiopaque overlay surrounding the aperture.

FIGS. 11A, 11B and 11C show three rotational orientations of a reentry zone support.

FIG. 11D is an exploded side elevational view of the reentry zone support of FIG. 11A.

FIG. 11E is a side elevational view of the support of FIG. 11A, in a curved configuration.

FIG. 12 is a cross sectional perspective view of a catheter shaft portion having separate guide wire and aspiration lumen.

FIG. 13 is a perspective view of a reentry zone having a mix of reentry ports and tissue stabilizing aspiration ports.

FIG. 14 illustrates different fluoroscopic visualization options.

5

FIG. 15 is a schematic illustration of a reentry catheter distal end having an active deflection mechanism.

FIG. 16 shows a steerable reentry catheter with integrated handle.

FIG. 17 schematically illustrates reentry zones in combination with a guidewire steering insert.

FIG. 18 is a schematic illustration of a reentry catheter distal end having one configuration of a rapid exchange lumen.

FIG. 19 is a side elevational view of the integrated handle.

FIG. 20 illustrates the use of the reentry catheter to accomplish a delivery into the subintimal space.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

Referring to FIG. 1, there is disclosed a catheter 10 in accordance with one aspect of the present invention. Although primarily described in the context of a reentry catheter with a single central lumen, catheters of the present invention can readily be modified to incorporate additional structures, such as permanent or removable column strength enhancing mandrels, two or more lumen such as to permit drug or irrigant infusion or to supply inflation media to an inflatable balloon, or combinations of these features, as will be readily apparent to one of skill in the art in view of the disclosure herein.

The catheters disclosed herein may readily be adapted for use throughout the body wherever it may be desirable to create an extravascular access or a neo lumen, such as to traverse a CTO or otherwise exit and reenter the lumen. For example, catheter shafts in accordance with the present invention may be dimensioned for use throughout the coronary and peripheral vasculature, the gastrointestinal tract, the urethra, ureters, Fallopian tubes and other lumens and potential lumens, as well.

The catheter 10 generally comprises an elongate tubular body 16 extending between a proximal end 12 and a distal functional end 14. The length of the tubular body 16 depends upon the desired application. For example, lengths in the area of from about 120 cm to about 160 cm or more are typical for use in femoral access percutaneous transluminal coronary applications. Intracranial or other applications may call for a different catheter shaft length depending upon the vascular access site, as will be understood in the art.

The proximal end 12 of catheter 10 is additionally provided with a manifold 18 having one or more access ports as is known in the art. Generally, manifold 18 is provided with a guidewire port 20 in an over-the-wire construction, and an optional side port 22 depending upon the desired functionality. Additional access ports may be provided as needed, depending upon the functional capabilities of the catheter. Manifold 18 may be injection molded from any of a variety of medical grade plastics, or formed in accordance with other techniques known in the art.

The tubular body 16 is provided with a reentry zone 40, extending between a proximal exit port 42 and a distal exit port 44, configured to permit exit of a guidewire there-through. Preferably at least three or five or seven or more exit ports or port pairs are provided, arranged circumferentially offset from each other so that regardless of the rotational orientation of the catheter in the vessel, at least one exit port will be facing the direction of the true vessel lumen. The exit ports may be arranged in a spiral, with axially adjacent ports rotated from each other about the longitudinal axis of the catheter within the range of from about 5 degrees

6

and 90 degrees, preferably between about 10 degrees and 60 degrees, and in some embodiments between about 15 degrees and 35 degrees.

In an axial direction, adjacent ports may be spaced apart by a distance within the range of from about 2 mm to about 4 mm or about 5 mm and about 15 mm. Side ports define a reentry zone 40 having an axial length from the proximal most port 42 to the distal most port 44 of at least about 2 mm and generally less than about 20 mm; in many implementations between about 4 mm and 15 mm. The side ports define a spiral that extends at least about 45 or 90 degrees around the catheter side wall but typically no more than about 360 degrees and in certain embodiments within the range of from about 270 degrees and 450 degrees.

Referring to FIG. 2 the coronary artery walls are made up of three main layers. The intima is the innermost layer consisting of a single layer of endothelial cells. The fibromuscular media includes nonstriated myocytes. The adventitia is the outermost layer composed of collagen and elastin.

The intima layer can thicken considerably over time, occluding the blood flow through the artery. A chronic total occlusion (CTO) is a complete blockage of the artery. The present invention relates to a method to treat a CTO by creating a new lumen in the subintimal space (between the adventitia and intima) in order to allow blood flow in the artery around the occlusion.

Referring to FIG. 3A, a guidewire 50 is advanced through the arterial lumen 52 to the proximal side of an obstruction to be treated such as a CTO 54. Progress of the wire 50 may be impeded or deflected due to the CTO. If the guidewire cannot cross the lesion, the guidewire may be passed distally beyond the lesion by way of an intentional dissection, and is advanced in a created subintimal channel between the intimal and medial layers of the arterial wall. This allows the guidewire 50 to cross the CTO 54 via the subintimal space. A reentry catheter 10 is then advanced over the guide wire 50, following the guidewire from the native arterial lumen, through the dissection and into the subintimal space. See FIG. 3B. The guidewire 50 may thereafter be retracted into the guide catheter.

As seen in more detail in FIG. 3C, the reentry catheter 10 exits the native lumen at a subintimal entry point 56, and travels distally within the subintimal space. The guide wire 50 may thereafter be advanced distally within the reentry catheter 10 and rotated to find the exit port having the desired axial and rotational orientation to direct the guidewire 50 towards the native vascular lumen 52. The guidewire may thereafter be distally advanced to exit through the selected exit port 58, distal of the lesion 54, for reentry into the native vascular lumen 52 at guidewire reentry point 60.

Once the guidewire 50 has correctly reentered the lumen distally of the CTO, the reentry catheter 10 can be proximally retracted from the subintimal space leaving the guidewire in position via the neo lumen across the CTO. See FIG. 3D. The reentry catheter can thereafter be withdrawn from the artery.

Any of a variety of procedures can be accomplished with the guidewire in position across the CTO. For example, referring to FIG. 3E, a balloon catheter 62 can be advanced over the guide wire 50 to position an inflatable balloon 64 in the subintimal space. Dilatation of the balloon can open a flow channel to cross the CTO via the subintimal space. The balloon may carry a balloon expandable stent 66 which can be expanded spanning the CTO to support the neo lumen against collapse following removal of the balloon as is understood in the art. Alternatively a self-expanding stent

may be deployed across the CTO, preferably following a mechanical dilatation (e.g., balloon dilatation step).

Additional details of the catheter design may be seen with reference to FIGS. 4A-5A. A plurality of successive axially spaced exit ports **46** are arranged in a spiral such as a helix about the longitudinal axis of the catheter. The guide wire **50** may have a pre-bent tip so that it is biased laterally against the inside diameter of the reentry catheter sidewall. The guide wire may be distally advanced and rotated to align, for example, with distal most exit port **44** and advanced through that port. See FIG. 4A.

Alternatively, if the native arterial lumen is in a different orientation relative to the reentry catheter **10**, the guide wire can be axially repositioned and rotated to align and exit via a second different exit port to reenter the arterial lumen at a different orientation as seen in FIG. 4B.

Referring to FIGS. 1 and 5A, the proximal most port **42** and distal most port **44** define reentry zone **40** along which a plurality of ports **46** will generally encompass at least about 270 and preferably about 360 degrees around the circumference of the reentry catheter **10**. Generally between about 4 and 16 ports are provided with one embodiment between about six and ten ports. A reentry zone **40** having eight ports aligned along a 360 degree spiral results in 45 degrees of rotation between adjacent ports. Preferably, ports are arranged in sets of opposing pairs, as is discussed further below.

Referring to FIG. 5B, the ports will generally have a major axis **80** extending longitudinally along the catheter and a minor, transverse axis extending circumferentially around the tubular body. The major axis will typically be within about 15 degrees or 10 degrees or less from parallel with the catheter longitudinal axis and may be about parallel to the longitudinal axis as shown in FIG. 5B, or aligned with the spiral on which the ports reside.

The major axis **80** is generally longer than the minor axis **82**, and may be at least about 150%, or 175% or 200% or more than the length of the minor axis **82**. In some implementations of a reentry catheter, the minor axis **82** is within the range of from about 0.012 inches to about 0.20 inches; or about 0.014 inches to about 0.018 inches. The major axis **80** is within the range of from about 0.024 inches to about 0.046 inches, or about 0.030 inches to about 0.042 inches. In one example, the port is about 0.016 by about 0.034 inches in a catheter having an OD of about 0.038 inches. The minor axis of the port may be less than about half of the tubular body OD and over about half of the catheter body ID.

Preferably, the ID of the tubular catheter body is at least about 120% or 150% or 175% or 200% or more of the OD of the GW intended to be used with the catheter. In one implementation, a catheter having an ID of about 0.028 inches is intended for use with a 0.014 inch guide wire. The difference between the diameter of the guide wire and the ID of the catheter is generally at least about 0.005 or about 0.010 or more, to facilitate manipulation of the guidewire and directing the guidewire towards a desired exit port.

In addition, the relatively large space between the guidewire and the ID of the catheter facilitates application of vacuum (e.g., up to about 29" Hg, or 20 mm Hg) while the guide wire is in position extending through the tubular body, which allows negative pressure applied to the central lumen to produce suction at the exit ports for anchoring the catheter to the adjacent tissue. Anchoring the reentry zone to adjacent tissue may be desirable to stabilize the catheter and facilitate penetration during the step of puncturing tissue with the guidewire to reenter the vessel lumen distally of the obstruction.

The exit ports **46** may be spaced apart axially by a distance within the range of from about 0.05 inches to about 0.25 inches or in some embodiments from about 0.08 inches to about 0.20 inches. Multi-sized ports can be provided, with a first set of guidewire exit ports and a second set of smaller aspiration ports arrayed among the guidewire ports. Multiple sizes of ports may also be utilized for infusion of therapeutic agents.

A variety of port geometries and ramp geometries may be utilized to optimize control over port selection and guidewire exit. Referring to FIG. 6A, the edge of the catheter wall at the distal end of a port **46** may be provided with a ramped surface **84** configured to facilitate exit of the guidewire. Alternatively, a ramp surface **84** may be provided by forming a tab **86** that inclines radially inwardly in a proximal direction into the lumen. A guidewire with a laterally biased tip can be rotated and advanced until the tip enters the port assisted by the ramp **84** on the sidewall or on a tab. See FIGS. 7A and 7B.

Deflection of the guidewire may also be facilitated by an intermediate deflection element such as a deflection guide **88**. See FIG. 8. The deflection guide **88** may comprise a shape memory (e.g., Nitinol) tube **90** that is preset to an angle upon proximal retraction of or distal advance from of a restraint.

Referring to FIG. 9, there is illustrated a reentry catheter **10** including a reentry zone support **92** extending throughout the reentry zone **40**. The support **92** includes a tubular body **94** extending between a proximal end **96** and a distal end **98** and which carries a plurality of exit ports **46** spaced apart by a plurality of intervening flexible links **47**. Additional detail is described in connection with FIGS. 10A-10E.

Extending proximally from the support **92** is a kink resistance and torque transmission feature such as a braided tubular sidewall component **186**. Braid **186** may be a stainless steel braid having between about 12 and 20 filaments, and in one implementation 16 rectangular filaments having a width that is at least about 3× or 4× the thickness. The braid may overlay a coil layer **188**, which in one implementation is a four filar coil of 0.001" tungsten wire at about 0.008" pitch. The braid **186** overlaps the proximal end of the support **92**, but in the illustrated implementation the distal end of the coil **188** is spaced proximally apart from the proximal end of the support **92**.

At least a first eyelet frame **100** comprising an annular strut **102** encircles a guidewire exit port or aperture **104** on a first side of the tubular body **94**. In the illustrated embodiment, the first eyelet frame **100** is spaced apart from the proximal end **96** by a first flexible link **106** in the form of an elongated helical strut **108**. Proximal end **96** is additionally provided with a plurality of anchors such as at least about four or six or eight or more proximally extending ribs **110**, for facilitating attachment to the outer surface of an underlying catheter body component such as a woven or braided reinforcement layer as shown in FIG. 10C.

A second eyelet frame **112** in the form of a second annular strut **114** defines a second aperture **116**. Second eyelet frame **112** is spaced distally apart from the first eyelet frame **100** by a second flexible link **118** in the form of a second helical strut **120**. The total number of apertures in a reentry zone on a particular reentry catheter can be varied depending upon the desired clinical performance, as has been discussed elsewhere here in.

Referring to FIG. 10D, the distal end of the reentry support **92** is provided with at least about four or six or eight or more tip anchors such as axially extending ribs **190**. Ribs **190** may be provided with a circumferential segment **192** to create an interference fit when embedded in the polymer of

the tip **194**, which may comprise 35D PEBAX. As shown in FIG. **10E**, selected portions of the reentry support may be provided with a radiopaque marker such as a radiopaque coating layer. In the illustrated embodiment, the annular struts or eyelets that define the ports are provided with a layer of radiopaque material such as a Pt/Ir alloy, allowing an opposing port pair to appear as an oval aperture when aligned with the viewing axis.

As seen in FIGS. **11A-C**, a six port implementation is shown in which each aperture on a first side of the tubular body is paired with a second opposing aperture on the opposite side of the tubular body to form first, second and third aperture pairs **130**, **132** and **134**. A support **92** viewed from the perspective of FIG. **11A** along an axis that extends at a perpendicular through each of the first and second windows **104A** and **104B** of the first aperture pair **130** appears under fluoroscopic visualization as a dark ring surrounding an opening, or an "O" or other indicium of a first rotational orientation.

The support **92** as shown in FIG. **11B** has been rotated about its longitudinal axis by 60° compared to FIG. **11A**. Viewed from the same viewing angle, the first aperture pair **130** is no longer aligned with the viewing axis so the window **104A** has visually disappeared. Instead a sidewall of the tubular body becomes opaque such as in the form of an "X" or other indicium of a second rotational orientation. The first and third aperture pairs **130**, **134** appear as an X or other indicium of non alignment. A further rotation of the support through an additional 60 degrees produces the view shown in FIG. **11C**, in which the visualized "O" has moved to the third aperture pair **134**.

Thus, the white "O" will progress along the length of the support from exit port pair to next adjacent exit port pair, as a function of rotational orientation. In this manner, the clinician can determine the rotational orientation of the distal end of the catheter under fluoroscopic visualization by tracking the location of the O and the X's relative to catheter rotation. This facilitates rotational alignment of the catheter relative to the true lumen, and selection of the appropriate exit port for launching the guidewire through the selected port and in the direction of the true lumen.

Referring to FIG. **11D**, there is illustrated an exploded view of the different functional components of the support. The components may be separately formed and connected such as by welding, or the entire assembly may be cut from a single piece of tubestock such as by laser cutting, EDM or other techniques known in the art.

Trackability and pushability are catheter characteristics that rely on the ability for the distal end of the catheter to push through the tortuous anatomy of the cardiac arteries. The consistency of the bending moments throughout the catheter shaft have significant impact on these use characteristics. The illustrated support insert comprises 9 discrete regions, labelled 1-9 in FIG. **11D**.

1. The proximal end is provided with a plurality of engagement structures such as at least two or four or six or more axially extending fingers designed to overlap and intertwine with the braid and coil reinforcement of the shaft

2. First, proximal, single or dual start, first direction such as clockwise spring section. This proximal spring section has the highest relative stiffness to account for the moment arm to the distal end of the catheter and enable the smooth, approximately constant radius curvature under lateral load, as seen in FIG. **11E**. This section is at least about 2x or 3x or preferably 4x stiffer than the distal end **9**. As illustrated, the spring section has 3 revolutions, 0.021" pitch, 0.0045" width.

3. First proximal port. Annular frame is configured to define an oblong port and opposing aperture pair to provide differing visual presentation under fluoroscopy indicative of rotational orientation. Dual exit locations are approximately 180 degrees rotated.

4. 2nd spring region may have a counterclockwise rotation to enhance torque response, and may also have a dual start. As illustrated, the second spring section has 4 revolutions, 0.014" pitch, 0.0040" width.

5. The middle port pair **132** is rotated 60 degrees from first port pair **130**. All other geometry of the three port pair frame segments are the same.

6. The third spring region may have about 4 revolutions, 0.014" pitch, 0.0030" width.

7. The distal port pair **134** is rotated 60 degrees from the middle port pair **132**.

8. The fourth spring region may be provided with between about three and 10 and in the illustrated embodiment six dual start revolutions, 0.0105" pitch, 0.0030" width

9. The distal end is provided with a plurality of anchors configured for maximum surface area to allow embedded anchoring within the soft tip material to intertwine with the metallic insert and increase tensile strength.

Any of the pitch and width dimensions provided above can be varied by +/-5%, 10% 15%, or 20% depending upon the desired performance.

Reinforcement of the apertures can be accomplished with multiple components that can articulate. Reinforcement may have spring like components for inter-connection. Material may be polymeric or metallic. Material may be radiopaque. Reinforcement will be layered within polymeric tubing to create a laminate structure. Ports may be cut through the braided regions before or after lamination. Multiple materials of construction may be used. Components may be welded together for robustness. Ports can be singulated (discrete components) and positioned in multiple orientations to optimize selection by the guidewire. Material may be polymeric or metallic. Ports can be single sided. Ports can be dual sided as illustrated.

One aspect of the invention involves aspiration via the side ports to secure adjacent tissue. Aspiration can be accomplished via the guidewire exit ports and/or separate aspiration ports.

For example, referring to FIG. **12**, there is illustrated a perspective cross section through a catheter body segment **150**, showing a guidewire lumen **152** in communication with at least one exit port **154**, and a separate aspiration lumen **156** in communication with at least one aspiration port **158**. In any of the embodiments disclosed herein, the aspiration lumen or guidewire lumen may also be used to infuse fluids which may include one or more drugs.

FIG. **13** illustrates a reentry catheter segment having relatively larger guidewire exit ports, and a plurality of smaller aspiration ports. Aspiration can be accomplished either via guidewire exit ports or dedicated aspiration ports. In either case, aspiration can reduce the blood volume in the neo lumen and or stabilize the wall of the neo lumen (intima) to facilitate puncture by the guidewire to facilitate reentry into the native lumen.

Blood aspiration flow rates, pressure may be controlled via an external vacuum source. Vacuum regulators may be provided to control flow rates, and absolute pressures. Guidewire Re-entry port design may also be used to aspirate blood during access into subintimal space. The vacuum source will be able to measure pressure differentials within the device. The vacuum source may be design as a stand-alone system or connected to a lab's vacuum source. Addi-

11

tionally, a pressure pump may be used as a vacuum source. Vacuum can be applied in a multitude of modes that are controlled by surgeon or automated. Pulsatile for effective aspiration of hematoma, pulsatile to allow axial advancement while removing hematoma, high pressure or low pressure pulsatile vacuum can be controlled by an automatic valve that pulses at a discrete or variable frequency

FIG. 14 shows different visualization schemes that may be employed. Preferably, the distal tip has high radiopacity to facilitate visualization. First and second marker bands are preferably positioned at the proximal and distal ends of the reentry zone. In one implementation, the reentry zone may be substantially radiolucent, and the frame surrounding each exit port is radiopaque.

The catheter shaft may be steerable bi-directionally or uni-directionality. The catheter shaft may have the ability to accumulate torque between the handle and the tip. The catheter may have the ability to advance in a way that 'taps' to facilitate tracking—axial extension and compression. All of these characteristics are to facilitate tracking through tortuous anatomy and facilitate traversing the subintimal plane.

Referring to FIGS. 15 and 16, there is illustrated a bidirectionally steerable catheter 10. A proximal control 160 such as a rotatable wheel or axial slider is in communication with a distal steering zone 162 by at least one and, as illustrated, two pull wires 164, 166. Manipulation of the control 160 to proximally retract the pull wire 166 will deflect the steering zone 162 in a first direction as illustrated. Proximal retraction of the second pull wire 164 will cause deflection of the steering zone 162 in a second, opposite direction.

Referring to FIG. 17, the design may optionally incorporate an internal steerable guide sheath 170 between the guidewire and the catheter shaft. Guide sheath includes a guidewire lumen 172 which terminates distally in a ramped surface to direct a guidewire through a lateral guide wire port 174. To prevent a physician from spinning a GW (trial and error) to get to a desired exit port, the sheath 170 will cover all holes except the desired re-entry port which is aligned with sheath port 174. The user may easily select the desired ports by localizing the ports under fluoroscopy and axially and rotationally adjusting the guide sheath to aim at the desired exit port.

Referring to FIG. 18, a dual-lumen catheter shaft may be provided to allow for a Rapid Exchange catheter design. A first, reentry guidewire may be advanced through the lumen accessed vial the proximal luer, and a second, navigational guidewire may be advanced through the second, rapid exchange lumen. In this configuration, the proximal exit port for the second, rapid exchange lumen will be located on a side of the catheter distally of the proximal luer, such as within about 40 cm or 30 cm or 20 cm of the distal end of the catheter.

The first lumen may also be used for aspiration while the second lumen may only be available for a guidewire. It may be desirable to isolate one or more lumens for aspiration, such as shown in FIG. 18. For example a one-way valve may permit passing of a guidewire but also close when the guidewire is removed to facilitate aspiration via the other lumen.

Referring to FIG. 19, the integrated handle may be connected to a power source (1) for therapeutic delivery while accessing the subintimal space. Power sources may include, for example, radio frequency generators for RF ablation or cryoablation generators, and a RF or cryo deliv-

12

ery element may be carried by the distal end of the catheter or by a removable catheter insert depending upon the desired functionality.

The integrated handle may also be connected to a vacuum source (2) for blood aspiration to prevent hematoma as well as assisting with device fixation within the subintimal space. The integrated device may include a vacuum accumulator within the handle that could interact with operator controls.

The integrated handle and one or two or more lumen extending throughout the catheter may also be configured to be compatible with a variety of commonly used tools for CTO crossing procedures, including guidewires, guide liners to increase stiffness for increase pushability, drilling microcatheters to gain access to the subintimal space; dilation balloon catheters; or infusion pumps for delivering therapeutic agents.

Referring to FIG. 20, the catheter 10 provides the ability to access the subintimal space and achieve a variety of additional advantages such as the ability to deliver drugs such as therapeutic agents to help heal dissections, anticoagulants, or contrast, or monitor ECG signals. In addition, the catheter enables delivery of a variety of devices 180, such as customized implants or sensors.

It may be desirable to coat the outside surface of the guidewire and/or the inside surface of the wall defining the guidewire lumen with a lubricious coating to minimize friction as the catheter 10 is axially moved with respect to the guidewire. A variety of coatings may be utilized, such as Paralene, Teflon, silicone rubber, polyimide-polytetrafluoroethylene composite materials or others known in the art and suitable depending upon the material of the guidewire or inner surface of the tubular wall.

In prior art intravascular catheters, the intended guidewire is normally configured to substantially occupy the guidewire lumen, with a minimal tolerance necessary to avoid excessive friction. For example, a catheter having a 0.018" ID guidewire lumen might be used with a 0.014" guidewire. The reentry guidewire of the present invention is preferably substantially smaller than the ID of the complementary lumen. For example, a 0.014" guidewire may be used with a catheter 10 having a 0.028" lumen. In general, the guidewire will have a diameter that is no more than about 80%, and preferably no more than about 70% or 60% of the ID of the corresponding lumen. This provides an aspiration flow path in the space between the guidewire and the lumen wall to enable aspiration of blood from the intraluminal space and anchoring of the catheter against adjacent tissue while the guidewire remains in place. For example, with a 0.014" guidewire present and a maximum vacuum pressure of 20 mmHg, at least about 6 mL/Min, and preferably at least about 8 mL/MIN or at least about 10 mL/min of saline or water or more is aspirated.

The catheters of the present invention may comprise any of a variety of biologically compatible polymeric resins having suitable characteristics when formed into the tubular catheter body segments. Exemplary materials include polyvinyl chloride, polyethers, polyamides, polyethylenes, polyurethanes, copolymers thereof, and the like. Optionally, the tubular body may further comprise other components, such as radiopaque fillers; colorants; reinforcing materials; reinforcement layers, such as braids and helical reinforcement elements; or the like. In particular, the tubular body may be reinforced such as with an embedded coil or one or two or more braided tubular layers in order to enhance its column strength and torqueability while preferably limiting its wall thickness and outside diameter. The tubular body 16 may be produced in accordance with any of a variety of known

13

techniques for manufacturing interventional catheter bodies, such as by extrusion of appropriate biocompatible polymeric materials.

Radiopaque markers may be provided at least at the distal end **25** and the proximal end of the reentry zone **40**. One suitable radiopaque marker comprises a metal band which is fully embedded within the catheter wall. Suitable marker bands can be produced from a variety of materials, including platinum, gold, and tungsten/rhenium alloy.

In many applications, the tubular body **16** is provided with an approximately circular cross-sectional configuration having an external diameter within the range of from about 0.025 inches to about 0.065 inches. In accordance with one embodiment of the invention, the proximal section of tubular body **16** has an external diameter of about 0.042 inches (3.2 f) throughout most of its length. Alternatively, a generally oval or flattened cross-sectional configuration can be provided in a distal zone, as well as other noncircular configurations, depending upon the desired performance.

In a catheter intended for peripheral vascular applications, at least the proximal section of body **16** will typically have an outside diameter within the range of from about 0.039 inches to about 0.110 inches. In coronary vascular applications, the proximal section of body **16** will typically have an outside diameter within the range of from about 0.025 inches to about 0.080 inches. The OD of the catheter may taper or step to a smaller diameter or dimension in a distal zone.

Diameters outside of the preferred ranges may also be used, provided that the functional consequences of the diameter are acceptable for the intended purpose of the catheter. For example, the lower limit of the diameter for any portion of tubular body **16** in a given application will be a function of the number of fluid or other functional lumen contained in the catheter, together with the acceptable minimum performance characteristics.

For example, referring to FIG. 9, a strain relief **182** may extend within the range of from about 25 mm to about 50 mm, or about 35 to about 40 mm from the proximal hub. The OD steps down from about 0.080" to about 0.041" (less than about 75% or 65% or less than about 55% of the OD of the strain relief **182** section of the catheter body) distally of transition **184**. The catheter body distally of transition **184** may include at least two or three zones of distinct flexibility. In a modified 3 point bend test, a) a distal most zone will preferably exert between about 6-10 gf when deflected 15 mm but less than 15 gf. An intermediate or mid shaft zone will preferably exert between about 10-20 gf when deflected 15 mm but less than 30 gf, and a proximal zone will preferably exert between about 30-60 gf when deflected 15 mm but less than 100 gf. Preferably, the catheter shaft will exert at least about 0.10 ozf-in at the metallic insert junction when rotated 360 but less than 1 ozf-in.

The proximal zone may have a length within the range of from about 850-1050 mm, and in some implementations from about 925 to about 975 mm. The intermediate zone may have a length within the range of from about 150 mm to about 250 mm, from about 175 mm to about 225 mm, or about 190 mm to about 210 mm. The distal zone may have a length within the range of from about 150 mm to about 250 mm, from about 180 mm to about 230 mm, or about 195 mm to about 220 mm.

Although the present invention has been described in terms of certain preferred embodiments, it may be incorporated into other embodiments by persons of skill in the art in

14

view of the disclosure herein. The scope of the invention is therefore not intended to be limited by the specific embodiments disclosed herein, but is intended to be defined by the full scope of the following claims.

Further variations and additional details of the catheters disclosed herein are disclosed in the attached Appendix, any one or combination of which may be combined with any of the features described above, depending upon the desired performance. The contents of the Appendix are hereby incorporated by reference in their entirety herein.

What is claimed is:

1. A reentry catheter for crossing a vascular occlusion, comprising:

an elongate flexible tubular body, having a proximal end, a distal end and at least one lumen extending there through;

a reentry zone on the tubular body, comprising at least six side wall exit apertures in communication with the lumen, the exit apertures arranged in three pairs of exit apertures axially spaced apart and each pair rotationally offset from an adjacent pair by an angle within a range of between about 10 degrees and 60 degrees; and

a radiopaque eyelet in the side wall surrounding each exit aperture, wherein the radiopaque eyelets are connected together by a frame in the side wall,

wherein the reentry zone is positioned within about 40 cm of the distal end of the tubular body.

2. A reentry catheter as in claim 1, wherein the reentry zone comprises at least four pairs of apertures, arranged in a spiral configuration around the tubular body.

3. A reentry catheter as in claim 1, wherein each pair of exit apertures is rotated 60 degrees with respect to each adjacent pair of apertures.

4. A reentry catheter as in claim 2, wherein at least one aperture has a noncircular configuration.

5. A reentry catheter as in claim 4, wherein at least one aperture has a major axis in parallel to a longitudinal axis of the tubular body, and a minor, transverse axis.

6. A reentry catheter as in claim 5, wherein at least one aperture has a minor axis diameter of at least about 0.014 inches.

7. A reentry catheter as in claim 6, wherein the major axis of the at least one aperture has a length of at least about 0.025 inches.

8. A reentry catheter as in claim 1, further comprising at least about four tip anchors.

9. A reentry catheter as in claim 1, wherein a portion of the frame comprises a helical strut extending between a first and second axially spaced apart opposing pairs of side wall exit apertures.

10. A reentry catheter as in claim 1, further comprising an inflatable balloon on the tubular body, in communication with a second, inflation lumen extending axially through the tubular body.

11. A reentry catheter as in claim 1, further comprising a guidewire lumen extending axially through the tubular body between a proximal port and a distal port.

12. A reentry catheter as in claim 11, wherein the proximal port is spaced distally apart from the proximal end of the tubular body.

13. A reentry catheter as in claim 12, wherein the proximal port is within about 20 cm of the distal end of the tubular body.

* * * * *